
urbs Documentation

Release 1.0.0

tum-ens

Dec 27, 2021

Contents

1	Contents	3
1.1	User's manual	3
1.1.1	Users guide	3
1.2	Mathematical documentation	22
1.2.1	Mathematical description	22
1.3	Technical documentation	49
1.3.1	Model Implementation	49
1.3.2	'urbs' module description	134
1.4	CoTraDis module	136
1.4.1	Coupling of Transmission and Distribution System Modules	136
2	Features	155
3	Changes	157
3.1	2019-03-13 Version 1.0	157
3.2	2017-01-13 Version 0.7	157
3.3	2016-08-18 Version 0.6	158
3.4	2016-02-16 Version 0.5	158
3.5	2015-07-29 Version 0.4	158
3.6	2014-12-05 Version 0.3	158
4	Screenshots	159
5	Dependencies	161
	Python Module Index	163
	Index	165

Author Johannes Dorfner, <johannes.dorfner@tum.de>

Organization Chair of Renewable and Sustainable Energy Systems, Technical University of Munich, <urbs@ens.ei.tum.de>

Version 1.0.0

Date Dec 27, 2021

Copyright The model code is licensed under the GNU General Public License 3.0. This documentation is licensed under a Creative Commons Attribution 4.0 International license.

1.1 User's manual

These documents give a general overview and help you getting started from after the installation (which is covered in the [README.md](#) file on GitHub) to you first running model.

1.1.1 Users guide

Welcome to urbs. The following sections will help you get started.

Overview model structure

urbs is a generator for linear energy system optimization models.

urbs consists of several **model entities**. These are commodities, processes, transmission and storage. Demand and intermittent commodity supply through are modelled through time series datasets.

Commodity

Commodities are goods that can be generated, stored, transmitted and consumed. By convention, they are represented by their energy content (in MWh), but can be changed (to J, kW, t, kg) by simply using different (consistent) units for all input data. Each commodity must be exactly one of the following six types:

- Stock: Buyable at any time for a given price. Supply can be limited per timestep or for a whole year. Examples are coal, gas, uranium or biomass.
- SupIm: Supply intermittent stands for fluctuating resources like solar radiation and wind energy, which are available according to a timeseries of values, which could be derived from weather data.

- **Demand:** These commodities have a timeseries for the requirement associated and must be provided by output from other process or from storage. Usually, there is only one demand commodity called electricity (abbreviated to Elec), but multiple (e.g. electricity, space heating, process heat, space cooling) demands can be specified.
- **Env:** The special commodity CO2 is of this type and represents the amount (in tons) of greenhouse gas emissions from processes. Its total amount can be limited, to investigate the effect of policies on the model.
- **Buy/Sell:** Commodities of these two types can be traded with an external market. Similar to Stock commodities they can be limited per hour or per year. As opposed to Stock commodities the price at which they can be traded is not fixed but follows a user defined time series.

Stock and environmental commodities have three numeric attributes that represent their price, total annual and per timestep supply or emission limit, respectively. Environmental commodities (i.e. CO2) have a maximum allowed quantity that may be created across the entire modeling horizon.

Commodities are defined over the tuple (year, site, commodity, type), for example (2020, 'Norway', 'Wind', 'SupIm') for wind in Norway with a time series or (2020, 'Iceland', 'Electricity', 'Demand') for an electricity demand time series in Iceland.

Process

Processes describe conversion technologies from one commodity to another. They can be visualised like a black box with input(s) (commodity) and output(s) (commodity). Process input and output ratios are the main technical parameters for processes. Fixed costs for investment and maintenance (per capacity) and variable costs for operation (per output) are the economical parameters.

Processes are defined over two tuples. The first tuple (year, site, process) specifies the location of a given process e.g. (2030, 'Iceland', 'Turbine') would locate a process Turbine at site Iceland. The second tuple (year, process, commodity, direction) then specifies the inputs and outputs for that process. For example, (2030, 'Turbine', 'Geothermal', 'In') and (2030, 'Turbine', 'Electricity', 'Out') describes that the process named Turbine has a single input Geothermal and the single output Electricity.

Transmission

Transmission allows instantaneous transportation of commodities between sites. It is characterised by an efficiency and costs, just like processes. Transmission is defined over the tuple (year, site in, site out, transmission, commodity). For example, (2030, 'Iceland', 'Norway', 'Undersea cable', 'Electricity') would represent an undersea cable for electricity between Iceland and Norway.

Storage

Storage describes the possibility to deposit a deliberate amount of energy in the form of one commodity at one time step; with the purpose of retrieving it later. Efficiencies for charging/discharging depict losses during input/output. Storage is characterised by capacities both for energy content (in MWh) and charge/discharge power (in MW). Both capacities have independent sets of investment, fixed and variable cost parameters to allow for a very flexible parametrization of various storage technologies; ranging from batteries to hot water tanks.

Storage is defined over the tuple (year, site, storage, stored commodity). For example, (2020, 'Norway', 'Pump storage', 'Electricity') represents a pump storage power plant in Norway that can store and retrieve energy in form of electricity.

Time series

Demand

Each combination (year, site, demand commodity) may have one time series, describing the aggregate demand (typically MWh) for a commodity within a given timestep. They are a crucial input parameter, as the whole optimization aims to satisfy these demands with minimal costs by the given technologies (process, storage, transmission). An additional feature for demand commodities is demand side management (DSM) which allows for the shifting of demands in time.

Intermittent Supply

Each combination (year, site, supim commodity) must be supplied with one time series, normalized to a maximum value of 1 relative to the installed capacity of a process using this commodity as input. For example, a wind power time series should reach value 1, when the wind speed exceeds the modeled wind turbine's design wind speed is exceeded. This implies that any non-linear behaviour of intermittent processes can already be incorporated while preparing this timeseries.

Buy/Sell prices

Each combination (year, Buy/sell commodity) must be supplied with one time series which represents the price for purchasing/selling the given commodities in the given modeled year.

Time variable efficiency

Each combination (year, site, process) can optionally be supplied with one time series which multiplies the outputs of the process with an according factor.

Get started

Welcome to urbs! Here you can learn how to use the program and what to do to create your own optimization problems and run them.

Inputs

There are two different types of inputs the user has to make in order to set up and solve an optimization problem with urbs.

First, there are the model parameters themselves, i.e. the parameters specifying the behavior of the different model entities such as commodities or processes. These parameters are entered into spreadsheets with a standardized structure. These then have to be placed in the subfolder `Input`. There can be no further information given on those parameters here since they make up the particular energy system

models. There are, however, two examples provided with the code, which are explained elsewhere in this documentation.

Second, there are the settings of the modeling run such as the modeling horizon or the solver to be employed. These settings are made in a run script. For the standard example such scripts are given named `runme.py` for the example `mimo-example` and `runBP.py` for the example `Business park`. To run a modeling run you then simply execute the according run script by typing:

```
$ python3 runscript.py
```

in the command prompt.

You can immediately test this after the installation by running one of the two standard examples using the corresponding example run scripts.

runscript explained

The runscript can be subdivided into several parts. These will be discussed here in detail.

Imports

The script starts with importing the relevant python libraries as well as the module `urbs`.

```
import os
import shutil
import urbs
```

The included packages have the following functions:

- `os` and `shutil` are builtin Python modules, included here for their data path and copying operations.
- `urbs` is the directory which includes the modules, whose functions are used mainly in this script. These are `prepare_result_directory()`, `setup_solver()` and `run_scenario()`.

More functions can be found in the document [API reference](#).

In the following sections the user defined input, output and scenario settings are described.

Input Settings

The script starts with the specification of the input files, which is either a single `.xlsx` file located in the same folder as the runscript or a collection of `.xlsx` files located in the subfolder `Input`:

```
input_files = 'Input'
result_name = 'Mimo-ex'
result_dir = urbs.prepare_result_directory(result_name) # name + time_
↳stamp

# copy input file to result directory
try:
    shutil.copytree(input_files, os.path.join(result_dir, 'Input'))
except NotADirectoryError:
```

(continues on next page)

(continued from previous page)

```
shutil.copyfile(input_files, os.path.join(result_dir, input_files))
# copy runme.py to result directory
shutil.copy(__file__, result_dir)
```

The input file/folder and the runscript are automatically copied into the result folder.

Next variables specifying the desired solver and objective function are set:

```
# choose solver (cplex, glpk, gurobi, ...)
solver = 'glpk'

# objective function
objective = 'cost' # set either 'cost' or 'CO2' as objective
```

The solver has to be licensed for the specific user, where the open source solver “glpk” is used as the standard. For the objective function urbs currently allows for two options: “cost” and “CO2” (case sensitive). In the former case the total system cost and in the latter case the total CO2-emissions are minimized.

The model parameters are finalized with a specification of timestep length and modeled time horizon:

```
# simulation timesteps
(offset, length) = (3500, 168) # time step selection
timesteps = range(offset, offset+length+1)
dt = 1 # length of each time step (unit: hours)
```

The variable `timesteps` is the list of timesteps to be simulated. Its members must be a subset of the labels used in `input_file`’s sheets “Demand” and “SupIm”. It is one of the function arguments to `create_model()` and accessible directly, so that one can quickly reduce the problem size by reducing the simulation length, i.e. the number of timesteps to be optimised. Variable `dt` is the duration of each timestep in the list in hours, where any positiv real value is allowed.

`range()` is used to create a list of consecutive integers. The argument `+1` is needed, because `range(a,b)` only includes integers from `a` to `b-1`:

```
>>> range(1,11)
[1, 2, 3, 4, 5, 6, 7, 8, 9, 10]
```

Output Settings

The desired output is also specified by the user in the runscript. It is split into two parts: reporting and plotting. The former is used to generate an excel output file and the latter for standard graphs.

Reporting

urbs by default generates an .xlsx-file as an ouput in `result_dir`. This file includes all commodities of interest to the user and can be specified as report tuples each consisting of a given year, sites and commodities combination. Information about these commodities is summarized both in sum (in sheet “Energy sums”) and as individual timeseries (in sheet “... timeseries”).

```
# detailed reporting commodity/sites
report_tuples = [
    (2019, 'North', 'Elec'),
    (2019, 'Mid', 'Elec'),
    (2019, 'South', 'Elec'),
    (2019, ['North', 'Mid', 'South'], 'Elec'),
    (2024, 'North', 'Elec'),
    (2024, 'Mid', 'Elec'),
    (2024, 'South', 'Elec'),
    (2024, ['North', 'Mid', 'South'], 'Elec'),
    (2029, 'North', 'Elec'),
    (2029, 'Mid', 'Elec'),
    (2029, 'South', 'Elec'),
    (2029, ['North', 'Mid', 'South'], 'Elec'),
    (2034, 'North', 'Elec'),
    (2034, 'Mid', 'Elec'),
    (2034, 'South', 'Elec'),
    (2034, ['North', 'Mid', 'South'], 'Elec'),
]
```

optional: define names for sites in report_tuples report_sites_name = {('North', 'Mid', 'South'): 'All'}

Optionally it is possible to define clusters of sites for aggregated information and with report_sites_name it is then possible to name these. If they are empty, the default value will be taken.

Plotting

urbs generates default result images. Which images exactly are desired can be set by the user. via the following input lines:

```
# plotting commodities/sites
plot_tuples = [
    (2019, 'North', 'Elec'),
    (2019, 'Mid', 'Elec'),
    (2019, 'South', 'Elec'),
    (2019, ['North', 'Mid', 'South'], 'Elec'),
    (2024, 'North', 'Elec'),
    (2024, 'Mid', 'Elec'),
    (2024, 'South', 'Elec'),
    (2024, ['North', 'Mid', 'South'], 'Elec'),
    (2029, 'North', 'Elec'),
    (2029, 'Mid', 'Elec'),
    (2029, 'South', 'Elec'),
    (2029, ['North', 'Mid', 'South'], 'Elec'),
    (2034, 'North', 'Elec'),
    (2034, 'Mid', 'Elec'),
    (2034, 'South', 'Elec'),
    (2034, ['North', 'Mid', 'South'], 'Elec'),
]

# optional: define names for sites in plot_tuples
plot_sites_name = {('North', 'Mid', 'South'): 'All'}

# plotting timesteps
```

(continues on next page)

(continued from previous page)

```
plot_periods = {
    'all': timesteps[1:]
}
```

The logic is similar to the reporting case discussed above. With the setting of plotting timesteps the exact range of the plotted result can be set. In the default case shown this range is all modeled timesteps. For larger optimization timestep ranges this can be impractical and instead the following syntax can be used to hard code which steps are to be plotted exactly.

```
# plotting timesteps
plot_periods = {
    'win': range(1000:1168),
    'sum': range(5000:5168)
}
```

In this example two 1 week long ranges are plotted between the specified time steps. Using this make sure, that the chosen ranges are subsets of the modeled time steps themselves.

The plot colors can be customized using the module constant `COLORS`. All plot colors are user-definable by adding color tuple() (r, g, b) or modifying existing tuples for commodities and plot decoration elements. Here, new colors for displaying import/export are added. Without these, pseudo-random colors are generated in `to_color()`.

```
# create timeseries plot for each demand (site, commodity) timeseries
for sit, com in prob.demand.columns:
```

Scenarios

This section deals with the definition of different scenarios. Starting from the same base scenarios, defined by the data in `input_file`, they serve as a short way of defining the difference in input data. If needed, completely separate input data files could be loaded as well.

The `scenarios` list in the end of the input file allows then to select the scenarios to be actually run.

```
scenarios = [
    urbs.scenario_base,
    urbs.scenario_stock_prices,
    urbs.scenario_co2_limit,
    urbs.scenario_co2_tax_mid,
    urbs.scenario_no_dsm,
    urbs.scenario_north_process_caps,
    urbs.scenario_all_together
]
```

The following scenario functions are specified in the subfolder `urbs` in script `scenarios.py`.

Scenario functions

A scenario is simply a function that takes the input data and modifies it in a certain way. with the required argument `data`, the input data `dict`:

```
# SCENARIOS
def scenario_base(data):
    # do nothing
    return data
```

The simplest scenario does not change anything in the original input file. It usually is called “base” scenario for that reason. All other scenarios are defined by 1 or 2 distinct changes in parameter values, relative to this common foundation.:

```
def scenario_stock_prices(data):
    # change stock commodity prices
    co = data['commodity']
    stock_commodities_only = (co.index.get_level_values('Type') == 'Stock')
    co.loc[stock_commodities_only, 'price'] *= 1.5
    return data
```

For example, `scenario_stock_prices()` selects all stock commodities from the `DataFrame` `commodity`, and increases their *price* value by 50%. See also pandas documentation [Selection by label](#) for more information about the `.loc` function to access fields. Also note the use of [Augmented assignment statements](#) (`*`=) to modify data in-place.:

```
def scenario_co2_limit(data):
    # change global CO2 limit
    hacks = data['hacks']
    hacks.loc['Global CO2 limit', 'Value'] *= 0.05
    return data
```

Scenario `scenario_co2_limit()` shows the simple case of changing a single input data value. In this case, a 95% CO2 reduction compared to the base scenario must be accomplished. This drastically limits the amount of coal and gas that may be used by all three sites.:

```
def scenario_north_process_caps(data):
    # change maximum installable capacity
    pro = data['process']
    pro.loc[('North', 'Hydro plant'), 'cap-up'] *= 0.5
    pro.loc[('North', 'Biomass plant'), 'cap-up'] *= 0.25
    return data
```

Scenario `scenario_north_process_caps()` demonstrates accessing single values in the `process DataFrame`. By reducing the amount of renewable energy conversion processes (hydropower and biomass), this scenario explores the “second best” option for this region to supply its demand.:

```
def scenario_all_together(data):
    # combine all other scenarios
    data = scenario_stock_prices(data)
    data = scenario_co2_limit(data)
    data = scenario_north_process_caps(data)
    return data
```

Scenario `scenario_all_together()` finally shows that scenarios can also be combined by chaining other scenario functions, making them dependent. This way, complex scenario trees can be written with any single input change coded at a single place and then building complex composite scenarios from those.

Run scenarios

This now finally is the function that gets everything going. It is invoked in the very end of the runscript.

```
for scenario in scenarios:
    prob = urbs.run_scenario(input_files, solver, timesteps, scenario,
                           result_dir, dt, objective,
                           plot_tuples=plot_tuples,
                           plot_sites_name=plot_sites_name,
                           plot_periods=plot_periods,
                           report_tuples=report_tuples,
                           report_sites_name=report_sites_name)
```

Having prepared settings, input data and scenarios, the actual computations happen in the function `run_scenario()` of the script `runfunctions.py` in subfolder `urbs`. It is executed for each of the scenarios included in the scenario list. The following sections describe the content of function `run_scenario()`. In a nutshell, it reads the input data from its argument `input_file`, modifies it with the supplied `scenario`, runs the optimisation for the given `timesteps` and writes report and plots to `result_dir`.

Reading input

```
# scenario name, read and modify data for scenario
sce = scenario.__name__
data = read_input(input_files, year)
data = scenario(data)
validate_input(data)
```

Function `read_input()` returns a dict `data` of up to 12 pandas DataFrames with hard-coded column names that correspond to the parameters of the optimization problem (like `eff` for efficiency or `inv-cost-c` for capacity investment costs). The row labels on the other hand may be freely chosen (like site names, process identifiers or commodity names). By convention, it must contain the six keys `commodity`, `process`, `storage`, `transmission`, `demand`, and `supim`. Each value must be a `pandas.DataFrame`, whose index (row labels) and columns (column labels) conforms to the specification given by the example dataset in the spreadsheet `mimo-example.xlsx`.

`data` is then modified by applying the `scenario()` function to it. To then rule out a list of known errors, that accumulate through growing user experience, a variety of validation functions specified in script `validate.py` in subfolder `urbs` is run on the dict `data`.

Solving

```
# create model
prob = urbs.create_model(data, dt, timesteps)

# refresh time stamp string and create filename for logfile
now = prob.created
log_filename = os.path.join(result_dir, '{}.log').format(sce)

# solve model and read results
optim = SolverFactory('glpk') # cplex, glpk, gurobi, ...
```

(continues on next page)

(continued from previous page)

```
optim = setup_solver(optim, logfile=log_filename)
result = optim.solve(prob, tee=True)
```

This section is the “work horse”, where most computation and time is spent. The optimization problem is first defined (`create_model()`) and populated with parameter values with values. The `SolverFactory` object is an abstract representation of the solver used. The returned object `optim` has a method `set_options()` to set solver options (not used in this tutorial).

The remaining line calls the solver and reads the `result` object back into the `prob` object, which is queried to for variable values in the remaining script file. Argument `tee=True` enables the realtime console output for the solver. If you want less verbose output, simply set it to `False` or remove it.

Business park example explained

In this part the input files of the standard example **Business park** will be explained in detail.

Task

The task we set ourselves here is to build our own intertemporal model. The task is the following:

The technical staff of a business park management company wants you to find the cost optimal energy system for their business park. You are to provide this with increasingly stricter CO2 emission limits over time. As the company expects to operate this business park for a long time still, they want you to help developing a long term strategy how to transform the energy supply infrastructure of the business park in cost optimal way over the time frame of 3 decades. The company also expects that the business park will be increasingly closely interacting with the neighboring small city and its energy system. All current and expected demand curves are given to you. You also have full access to regional climate models and all relevant parameters for the energy conversion units relevant for your problem.

Input files

The task set is intertemporal. That is we need to provide several `.xlsx` input files, one for each modeled year. Here we chose to use 3 files representing modeled years 10 years apart. For the given task this seems to be a good compromise between accuracy and computational effort. The files are named `2020.xlsx`, `2030.xlsx` and `2040.xlsx` and sit in the folder `Input (Business park)`. We will now proceed with a detailed walkthrough of the individual files.

Sheet Global

Here you can now specify the global properties needed for the modeling of the energy system. Note that this sheet has different entries for the different input files:

- **Support timeframe** (All files): Give the value for the modeled year here.
- **Discount rate** (Only first file): This value gives the discount rate that is used for intertemporal planning. It stands for the annual devaluation of money across the modeling horizon. In the example a discount rate of 3 % is used.

- **CO2 limit** (All files): This parameter limits the CO2 emissions across all sites within one modeled year, the *CO2 budget* sets a cap on the total emissions across all sites in the entire modeling horizon. If no restriction is desired enter 'inf' here. In the example increasingly strict values for the CO2 limit are used for the different modeled years, from 60 kt/a in 2020 over 45 kt/a in 2030 to 30 kt/a in 2040. This represents the will of the company to achieve milestones in the emission reductions while gradually changing their energy infrastructure.
- **CO2 budget** (Only first file): While the *CO2 limit* specified for each year limits the CO2 emissions across all sites within one modeled year, the *CO2 budget* sets a cap on the total emissions across all sites in the entire modeling horizon. If no restriction is desired enter 'inf' here. The *CO2 budget* is only active when the *Objective* is set to its default value 'cost'. In the example a CO2 budget of 1.2 Mt is used. This budget imposes a stricter limit on the emissions than the combined targets for the individual modeled year. In terms of climate impact this limit is the more important one. For all CO2 limitations the business park and the city are considered together since in the assumed case the company running the business park wants to act as an electricity provider for the city as well.
- **Cost budget** (Only first file): With this parameter a limit on the total system cost over the entire modeling horizon can be set. If no restriction is desired enter 'inf' here. The *Cost budget* is only active when the *Objective* is set to the value 'CO2'. In the example no CO2 optimization is considered this parameter is thus set to infinity.
- **Last year weight** (Only last file): In intertemporal modeling each modeled year is repeated until the next modeled year is reached. This is done by assigning a weight to the costs accrued in each of the modeled years. For the last modeled year the number of repetitions has to be set by the user here, where a high number leads to a stronger weighting of the last modeled year, i.e. of the final energy system configuration. In the example the last year has a weight of 10 years. This means that it will be equally weighted identically to the others which always represent all years until the next modeled year.

Sheet Site

In this sheet you can specify the site names and also the area of each site. The line index represents all the sites. The only site specific property to be set is then:

- **Area**: Specifies the usable area for processes in the given site. The area does not need to be the total floor area. It is used to limit the use of area consuming processes and can be seen as, e.g., the roof area for solar technologies.

In the example two sites 'Business park' and 'City' are given. These and their respective areas do not change. The areas here represent roof areas for PV and the city has more of this.

Sheet Commodity

In this sheet all the commodities, i.e. energy or material carriers, are specified. The line index completes a commodity tuple, i.e. a connection (year, site, commodity, type). There are three properties to be specified for all commodities of types **Stock**, **Buy**, **Sell** and **Environmental**.

- **Price** denotes the cost of taking one unit of energy from the stock for **Stock** commodities or emitting one unit of **Environmental**. For **Buy** and **Sell** commodities this is not directly a price but a multiplier for the time series given in the sheet 'Buy-Sell-Price'. It is thus typically set to 1 for these commodity types.

- **max** limits the total amount of the commodity that may be bought, sold or emitted per year.
- **maxperhaour** limits the total amount of the commodity that may be bought, sold or emitted per hour (not timestep but really hour).

In the site ‘Business park’ there are 9 commodities defined:

- *Solar (West/East)* is of type **SupIm** and represents the capacity factor timeseries of solar panels mounted with a given inclination (10° both West and East).
- *Grid electricity* is of type **Buy** and represents the electricity price as bought from the regional grid operator. The business park pays constant price over the year. In the site ‘City’ this price is different and hence a multiplier is used to increase the wholesale price for households.
- *Gas* is of type **Stock** and represents the price for the purchase of natural gas from the local provider.
- *Electricity, Heat and Cooling* are of type **Demand** and represent the hourly demand for these three energy carriers.
- *Intermediate* is of type **Stock**. However, it is not possible to buy this commodity from the stock. It is introduced to allow for a flexible operation of a combined heat and power (CHP) plant according to section *Modeling nuggets*.
- *Intermediate low temperature* is of type **Stock**. It is also not buyable from an external source. Its purpose is to make the operation of the cooling processes more realistic by preventing the storage of high temperature cooling from ambient air cooling in cold storages.

In site ‘City’ one additional commodity, *Operation decentral units* is introduced. It is of type **SupIm** and makes sure that the different heating technologies usable in the site all operate at a fixed share of the total heat demand. This is necessary, since these technologies are build up in a decentral way in the individual houses. The idea behind this is laid out in section *Modeling nuggets*.

Sheet Process

In this sheet the energy conversion technologies are described. Here only the economical and some general technical parameters are set. The interactions with the commodities are introduced in the next sheet. The following parameters are set here for the processes:

- **Installed capacity (MW) (Only first file)** gives the capacity of the process that is already installed at the start of the modeling horizon.
- **Lifetime of installed capacity (years) (Only first file)** gives the rest lifetime of the installed processes in years. A process can be used in a modeled year y still if the lifetime plus the first modeled year exceeds the next year $y+1$.
- **Minimum capacity (MW)** denotes a capacity target that has to be met by the process in a given modeled year. This means that the system will build at least this capacity.
- **Maximum capacity (MW)** restricts the capacity that can be built to the specified value.
- **Maximum power gradient (1/h)** restricts the ramping of process operational states, i.e. the change in the throughput variable. The value gives the fraction of the total capacity that can be changed in one hour. A value of 1 thus restricts the change from idle to full operational state (or vice versa) to at least a duration of one hour.

- **Minimum load fraction** gives a lower limit for the operational state of a process as a fraction of the total capacity. It is only relevant for processes where part-load behavior is modeled. A value here is only active when 'Ratio-Min' is numerical for at least one input commodity.
- **Investment cost (€/MW)** denotes the capacity specific investment costs for the process. You should give the book value here. The program will then translate this into the correct total, discounted cost within the model horizon.
- **Annual fix costs (€/MW)** represent the amount of money that has to be spent annually for the operation of a process capacity. They can represent, e.g., labour costs or calendaric ageing costs.
- **Variable costs (€/MWh)** are linked to the operation of a process and are to be paid for each unit of throughput through the process. They can represent anything from usage ageing to taxes.
- **Weighted average cost of capital** denotes the interest rate or expected return on investment with which the investor responsible for the energy system calculates.
- **Depreciation period** denotes both the economical and technical lifetime of all units in the system. It thus determines two things: the total costs of a given investment and the end of operational time for all units in the energy system modeled.
- **Area use per capacity (m^2/MW)** specifies the physical area a given process takes up at the site it is built. This can be used, e.g. to restrict the capacity of solar technologies by a total maximal roof area. The restricting area is defined in sheet 'Site'.

While the details of the processes will be discussed in more detail in the next section one mention on the processes 'Load dump' and 'Slack' is made here. These processes are not introduced to represent real units but help making operation more realistic and error fixing more easy. A load dump process just destroys energy which is sometimes necessary in order to prevent the system from doing unrealistic gymnastics to keep the vertex rule. A 'Slack' process can create a demand commodity out of thin air for an extremely high price. It thus indicates when the problem is not feasible, making error fixing much easier. Both should typically be included in models.

Sheet Process-Commodity

In this sheet the technical properties of processes are set. These properties are given for each process independent of the site where the process is located. You need to make an input for all the processes defined in the 'Process' sheet. The line index is a tuple (process, commodity, direction), where 'Direction' has to be set as either 'In' or 'Out' and specifies whether a commodity is an in- or an output of a given process. Under the column 'ratio' you then have to specify the commodity in- or outflows per installed capacity and time step at the point of full operation. The efficiency of the process for the conversion of one input into one output commodity is then given by the ratio of the chosen values. For example, in the modeled year 2020 the process 'Gas engine power plant' converts 2.2 MWh of 'Gas' into one MWh each of 'Electricity' and 'Heat' while emitting 0.2 t of 'CO2'. This corresponds to an efficiency of 0.45 for 'Heat' and 'Electricity' conversion.

If a process has a more complex part load behavior, where, e.g., the efficiency changes this can be partly captured by setting values in the 'ratio-min' column. These specify the commodity flows at the minimum operation point specified in the 'Process' sheet under 'min-fract'. The process will then no longer be allowed to turn off so use this carefully. In the present case this behavior is set for the combined heat and power plant 'CHP (Operational state)' only.

There are a few special settings made in the example. First, the CHP plant is divided into three parts. The idea behind this is described in [Modeling nuggets](#). The two processes 'CHP (Electricity driven)' and 'CHP (Heat driven)' specify the commodity flows in the two extreme operational states. The system can

then chose all linear interpolations between both states by guiding the commodity flow of ‘Intermediate’ through the two processes in the desired ratio. Second, the cooling technologies are implemented in a two stage way. The reason for this is that the process ‘Ambient air cooling’ is extremely efficient and extremely cheap. While it can only be used in certain time intervals (see explanation of ‘TimeVarEff’ further below), its output could nevertheless be stored otherwise which is not realistic. The introduction of commodity ‘Intermediate low temperature’ prevents this. It is the output of all the cooling technologies except for ‘Ambient air cooling’ and is also the one that can be stored (see below).

Sheet Transmission

In this sheet the parameters for transmission lines between sites are specified. The line index is part of a transmission tuple (`Site In`, `Site Out`, `Transmission`, `Commodity`). Note that for each transmission the inverse one with the same properties should also be given. The parameters are the following:

- **Efficiency (I)** specifies the transport efficiency of the transmission line.
- **Lifetime of installed capacity (years) (Only first file)** gives the rest lifetime of the installed transmission lines in years. A transmission line can be used in a modeled year y still if the lifetime plus the first modeled year exceeds the next year $y+1$.
- **Investment cost (€/MW)** denotes the capacity specific investment costs for the transmission line. You should give the book value here. The program will then translate this into the correct total, discounted cost within the model horizon.
- **Annual fix costs (€/MW)** represent the amount of money that has to be spent annually for the operation of a transmission capacity. They can represent, e.g., labour costs or calendaric ageing costs.
- **Variable costs (€/MWh)** are linked to the operation of a given transmission line.
- **Installed capacity (MW) (Only first file)** gives the transmission capacity of transmission lines already installed at the start of the modeling horizon.
- **Minimum capacity (MW)** denotes a transmission capacity target that has to be met by the transmission lines in a given modeled year. This means that the system will build at least this transmission capacity.
- **Maximum capacity (MW)** restricts the transmission capacity that can be built to the specified value.
- **Weighted average cost of capital** denotes the interest rate or expected return on investment with which the investor responsible for the energy system calculates.
- **Depreciation period** denotes both the economical and technical lifetime of all units in the system. It thus determines two things: the total costs of a given investment and the end of operational time for all units in the energy system modeled.

In the example the only commodity that can be transported from one site to the other is electricity.

Sheet Storage

In this sheet the parameters for storage units are specified. Each storage unit is indexed with parts of a storage tuple (`storage`, `commodity`). In storages charging/discharging power and the capacity are sized independently. The parameters specifying the storage properties are the following:

- **Installed capacity (MWh) (Only first file)** gives the storage capacity of storages already installed at the start of the modeling horizon.
- **Installed storage power (MW) (Only first file)** gives the charging/discharging power of storages already installed at the start of the modeling horizon.
- **Lifetime of installed capacity (years) (Only first file)** gives the rest lifetime of the installed storages in years. A storage can be used in a modeled year y still if the lifetime plus the first modeled year exceeds the next year $y+1$.
- **Minimum storage capacity (MWh)** denotes a storage capacity target that has to be met by the storage in a given modeled year. This means that the system will build at least this capacity.
- **Maximum storage capacity (MWh)** restricts the storage capacity that can be built to the specified value.
- **Minimum storage power (MW)** denotes a storage charging/discharging power target that has to be met by the storage in a given modeled year. This means that the system will build at least this power.
- **Maximum storage power (MW)** restricts the storage charging/discharging that can be built to the specified value.
- **Efficiency input (1)** specifies the charging efficiency of the storage.
- **Efficiency output (1)** specifies the discharging efficiency of the storage.
- **Investment cost capacity (€/MWh)** denotes the storage capacity specific investment costs for the storage. You should give the book value here. The program will then translate this into the correct total, discounted cost within the model horizon.
- **Investment cost power (€/MW)** denotes the storage charging/discharging power specific investment costs for the storage. You should give the book value here. The program will then translate this into the correct total, discounted cost within the model horizon.
- **Annual fix costs capacity (€/MWh)** represent the amount of money that has to be spent annually for the operation of a storage capacity. They can represent, e.g., labour costs or calendaric ageing costs.
- **Annual fix costs power (€/MW)** represent the amount of money that has to be spent annually for the operation of a storage power. They can represent, e.g., labour costs or calendaric ageing costs.
- **Variable costs capacity (€/MWh)** are linked to the operation of a given storage state, i.e. they lead to costs whenever a storage has a non-zero state of charge. These costs should typically set to zero but can be used to manipulate the storage duration or model state-of-charge dependent ageing.
- **Variable costs power (€/MWh)** are linked to the charging and discharging of a storage. Each unit of commodity leaving the storage requires the payment of these costs.
- **Weighted average cost of capital** denotes the interest rate or expected return on investment with which the investor responsible for the energy system calculates.
- **Depreciation period** denotes both the economical and technical lifetime of all units in the system. It thus determines two things: the total costs of a given investment and the end of operational time for all units in the energy system modeled.
- **Initial storage state** can be used to set the state of charge of a storages in the beginning of the modeling time steps. If *nan* is given this value is an optimization variable. In any case the storage

content in the end is the same as in the beginning to avoid windfall profits from simply discharging a storage.

- **Discharge** gives the hourly discharge of a storage. Over time, when no charging or discharging occurs, the storage content will decrease exponentially.

In the example there are no storages in site ‘City’ and there is a storage for each demand in site ‘Business park’. The commodity ‘Cooling’ is not directly storable to avoid an unrealistic behavior for the process ‘Ambient air cooling’ as was discussed above in the ‘Process-Commodity’ section.

Sheets Demand, SupIm, Buy/Sell price

In these sheets the time series for all the demands, capacity factors of processes using commodities of type ‘SupIm’ and market prices for ‘Buy’ and ‘Sell’ commodities are to be specified. For the former two the syntax ‘site.commodity’ has to be used as a column index to specify the corresponding tuple.

Sheet TimeVarEff

In this sheet a time series for the output of processes can be given. This is always useful, when processes are somehow dependent on external parameters. The syntax to be used to specify which process is to be addressed by this is ‘site.process’. In the present example, this is used for the process ‘Ambient air cooling’ which has a boolean ‘TimeVarEff’ curve giving the value ‘1’ for temperatures below a threshold and ‘0’ else.

This concludes the input generation. Of course all parameters have to be set in all the input sheets.

Run script

To run the example you can make a copy of the file `runme.py` calling it, e.g., `run_BP.py` in the same folder. You now just have to make 3 modifications. First, replace the report tuples by:

```
report_tuples = [
    (2020, 'Business park', 'Electricity'),
    (2020, 'Business park', 'Heat'),
    (2020, 'Business park', 'Cooling'),
    (2020, 'Business park', 'Intermediate low temperature'),
    (2020, 'Business park', 'CO2'),
    (2030, 'Business park', 'Electricity'),
    (2030, 'Business park', 'Heat'),
    (2030, 'Business park', 'Cooling'),
    (2030, 'Business park', 'Intermediate low temperature'),
    (2030, 'Business park', 'CO2'),
    (2040, 'Business park', 'Electricity'),
    (2040, 'Business park', 'Heat'),
    (2040, 'Business park', 'Cooling'),
    (2040, 'Business park', 'Intermediate low temperature'),
    (2040, 'Business park', 'CO2'),
    (2020, 'City', 'Electricity'),
    (2020, 'City', 'Heat'),
    (2020, 'City', 'CO2'),
    (2030, 'City', 'Electricity'),
    (2030, 'City', 'Heat'),
```

(continues on next page)

(continued from previous page)

```
(2030, 'City', 'CO2'),
(2040, 'City', 'Electricity'),
(2040, 'City', 'Heat'),
(2040, 'City', 'CO2'),
(2020, ['Business park', 'City'], 'Electricity'),
(2020, ['Business park', 'City'], 'Heat'),
(2020, ['Business park', 'City'], 'CO2'),
(2030, ['Business park', 'City'], 'Electricity'),
(2030, ['Business park', 'City'], 'Heat'),
(2030, ['Business park', 'City'], 'CO2'),
(2040, ['Business park', 'City'], 'Electricity'),
(2040, ['Business park', 'City'], 'Heat')
(2040, ['Business park', 'City'], 'CO2'),
]

# optional: define names for sites in report_tuples
report_sites_name = {('Business park', 'City'): 'Together'}
```

and the plot tuples by:

```
plot_tuples = [
    (2020, 'Business park', 'Electricity'),
    (2020, 'Business park', 'Heat'),
    (2020, 'Business park', 'Cooling'),
    (2020, 'Business park', 'Intermediate low temperature'),
    (2020, 'Business park', 'CO2'),
    (2030, 'Business park', 'Electricity'),
    (2030, 'Business park', 'Heat'),
    (2030, 'Business park', 'Cooling'),
    (2030, 'Business park', 'Intermediate low temperature'),
    (2030, 'Business park', 'CO2'),
    (2040, 'Business park', 'Electricity'),
    (2040, 'Business park', 'Heat'),
    (2040, 'Business park', 'Cooling'),
    (2040, 'Business park', 'Intermediate low temperature'),
    (2040, 'Business park', 'CO2'),
    (2020, 'City', 'Electricity'),
    (2020, 'City', 'Heat'),
    (2020, 'City', 'CO2'),
    (2030, 'City', 'Electricity'),
    (2030, 'City', 'Heat'),
    (2030, 'City', 'CO2'),
    (2040, 'City', 'Electricity'),
    (2040, 'City', 'Heat'),
    (2040, 'City', 'CO2'),
    (2020, ['Business park', 'City'], 'Electricity'),
    (2020, ['Business park', 'City'], 'Heat'),
    (2020, ['Business park', 'City'], 'CO2'),
    (2030, ['Business park', 'City'], 'Electricity'),
    (2030, ['Business park', 'City'], 'Heat'),
    (2030, ['Business park', 'City'], 'CO2'),
    (2040, ['Business park', 'City'], 'Electricity'),
    (2040, ['Business park', 'City'], 'Heat')
    (2040, ['Business park', 'City'], 'CO2'),
]
```

(continues on next page)

(continued from previous page)

```
# optional: define names for sites in plot_tuples
plot_sites_name = (('Business park', 'City'): 'Together')
```

In this way you get a meaningful output for the optimization runs. Second, the scenarios are made for the other example and are as such no longer usable here. Thus only the base scenario is to be run. Change the list scenario to the following:

```
scenarios = [
    urbs.scenario_base
]
```


Having completed all these steps you can execute the code.

Modeling nuggets

Here you can find a collection of non-trivial modeling ideas that can be used in linear energy system modeling with urbs. It is meant for more advanced users and you should fully understand the two standard examples **mimo-example** and **Business park** before proceeding. What follows is a loose collection of modeling approaches and does not follow any internal logic.

Different operational modes

For many power plants as, e.g., combined heat and power plants (CHP) there are different modes of operation. These and intermediate states between the extremes can be well captured in urbs models using the approach sketched in the following picture:

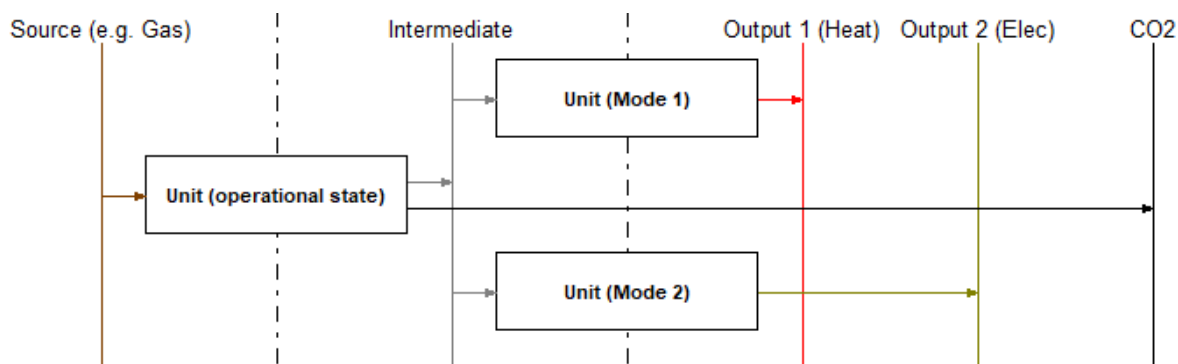

Here the vertical lines represent the commodities and the rectangle are processes. The arrows indicate in- and output commodities of the processes. In the case shown the power plant ‘Unit’ would be able to operate between a state where only ‘Output 1’ comes out and a state where only ‘Output 2’ comes out. The two extreme cases can, however, also be chosen as combinations of both outputs already.


The idea behind the figure is the following: The commodity ‘Intermediate’ is to be produced exclusively by the process ‘Unit (operational state)’. It thus simply tracks the throughput of this process. Due to the vertex rule (Kirchhoff’s current law) the commodity ‘Intermediate’ once produced needs to be consumed immediately. This can happen either via ‘Unit (Mode 1)’, ‘Unit (Mode 2)’ or a linear combination of both. The result is then the desired choice for the optimizer between states formed by linear combinations of the two modes. The commodity ‘Intermediate’ is best chosen as a **Stock** commodity where either the price is set to infinity or the maximum allowed usage per hour, or year (or both) is set to zero. This ensures that the commodity has to be produced by the process and cannot be bought from an external source, which for the present case would of course be absurd.

All process parameters and the setting of part load, time variable efficiency etc. is best done for the ‘Unit (operational state)’ process. The two other processes should in turn be used as mathematical entities that are defined by their ‘process commodity’ input only.

Proportional operation

Often many individual consumers are lumped together in one site. If a demand of these consumers is then met by a collection of decentral units it is important that the different technology options for these decentral units each fulfill a fixed fraction of the demand in each time step. This means that the different technology options are proportional to each other and the demand.

This behavior can be enforced by the following design:

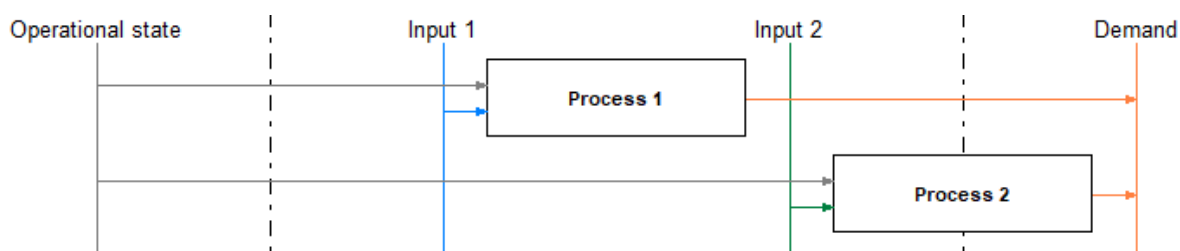

Here the vertical lines represent the commodities and the rectangle are processes. The arrows indicate in- and output commodities of the processes.

For the desired result the commodity ‘Operational state’ has to be of type **SupIm** and the corresponding time series has to be set as the normalized demand. In this way the optimizer can still size the two technology options ‘Process 1’ and ‘Process 2’ optimally while being forced to operate them proportionally to each other and to the demand. Other input or output (not shown) commodities can then be associated with the process operation as usual and will be dragged along by the forced operation.

Scenario generation

For a sensitivity analysis, it might be helpful to not manually create all scenario definitions automatically. For example, if one is interested in how installed capacities of PV and storage change the output, one might define ranges for each capacity. If there are four thresholds for the PV capacity and five for storage capacity, creating all 20 scenarios by hand is quite tiresome.

In this example, one wants to run an optimization with capacities 20 GW, 30 GW, 40 GW and 50 GW for PV and 50 GW, 60 GW, 70 GW, 80 GW and 90 GW for storage capacities.

Therefore, a function factory is created, which takes the values for PV and storage capacity and creates a scenario function out of it. This is done in the file *scenarios.py*:

```
def create_scenario_pv_sto(pv_val, sto_val):
    def scenario_pv_sto(data):
        # set PV capacity for all sites
        pro = data['process']
        solar = pro.index.get_level_values('Process') == 'Photovoltaics'
        pro.loc[solar, 'inst-cap'] = pv_val
        pro.loc[solar, 'cap-up'] = sto_val

        # set storage content capacity
        sto = data['storage']
```

(continues on next page)

(continued from previous page)

```
    for site_sto_tuple in sto.index:
        sto.loc[site_sto_tuple, 'inst-cap-c'] = sto_val
        sto.loc[site_sto_tuple, 'cap-up-c'] = sto_val

    return data
    # define name for scenario dependent on pv and storage values
    scenario_pv_sto.__name__ = f"scenario_pv{int(pv_val/1000)}_sto{int(sto_
    ↪val/1000)}"
    return scenario_pv_sto
```

In *runme.py* the following has to be added:

```
# define range for sensitivity
pv_vals = range(20000, 50001, 10000)
sto_vals = range(50000, 90001, 10000)

# create scenario functions
scenarios = []
for pv_val in pv_vals:
    for sto_val in sto_vals:
        scenarios.append(urbs.create_scenario_pv_sto(pv_val, sto_val))
```

1.2 Mathematical documentation

Continue here if you want to understand the theoretical conception of the model generator, the logic behind the equations and the structure of the features.

1.2.1 Mathematical description

In this Section the **mathematical description** of a model generated by urbs will be explained. The structure here follows the basic code structure and proceeds as follows:

First, a short introduction into the type of optimization problem solvable with urbs is given. This is followed by the description of the minimal possible model in urbs. As a next step the two main expansions of models, which also increase the index depth of all variables and parameters are discussed in the parts ‘Intertemporal modeling’ and ‘Multinode modeling’. The description is then concluded by the additional description of various feature modules. The latter are discussed in full index depth, i.e., with all features introduced in minimal, intertemporal and multinode modeling.

Structure of an urbs model

urbs is an abstract generator for linear optimization problems. Such problems can in general be written in the following standard form:

$$\begin{aligned} \min \quad & c^T x \\ \text{s.t.} \quad & Ax = b \\ & Bx \leq d. \end{aligned}$$

where x is the variable vector, c the coefficient vector for the objective function and A and B the matrices for the equality and inequality constraints, respectively. The equality constraints could also

be represented by inequality constraints, which is not done here for simplicity reasons. There are two options for the objective function: either the total system costs or environmental emissions can be used. The structure of the following parts will be first a description of x and c and subsequently a general formulation of the constraint functions that make up the matrices A and B as well as the vectors b and d . All variables and equations will be first presented for a minimally complex problem and the optional additional variables and equations are presented in extra parts.

Energy system entities

For all models that can be generated with urbs, the energy system is built up out of the following entities:

- Commodities, which represent the various forms of material and energy flows in the system.
- Processes, which convert commodities from one type to another. These entities are always multiple-input/multiple-output (mimo) that is, a certain fixed set of input commodities is converted into another fixed set of output commodities.
- Transmission lines, that allow for the transport of commodities between the modeled spatial vertices.
- Storages, which allow the storage of a single type of commodity.
- DSM potentials, which make the time shifting of demands possible.

Minimal optimization model

The minimal model in urbs is a simple expansion and dispatch model with only processes being able to fulfill the given demands. All spatial information is neglected in this case. The minimal model is already multiple-input/multiple output (mimo) and the variable vector takes the following form:

$$x^T = (\zeta, \underbrace{\rho_{ct}}_{\text{commodity variables}}, \underbrace{\kappa_p, \hat{\kappa}_p, \tau_{pt}, \epsilon_{cpt}^{\text{in}}, \epsilon_{cpt}^{\text{out}}}_{\text{process variables}}).$$

Here, ζ represents the total annualized system cost, ρ_{ct} the amount of commodities c taken from a virtual, infinite stock at time t , κ_p and $\hat{\kappa}_p$ the total and the newly installed process capacities of processes p , τ_{pt} the operational state of processes p at time t and $\epsilon_{cpt}^{\text{in}}$ and $\epsilon_{cpt}^{\text{out}}$ the total inputs and outputs of commodities c to and from process p at time t , respectively.

Objective

For any urbs problem as the objective function either the total system costs or the total emissions of CO2 can be chosen. In the former (standard) case this leads to an objective vector of:

$$c = (1, 0, 0, 0, 0, 0, 0),$$

where only the costs are part of the objective function. For the latter choice of objective no such simple structure can be written.

Costs

In the minimal model the total cost variable can be split into the following sum:

$$\zeta = \zeta_{\text{inv}} + \zeta_{\text{fix}} + \zeta_{\text{var}} + \zeta_{\text{fuel}} + \zeta_{\text{env}},$$

where ζ_{inv} are the annualized invest costs, ζ_{fix} the annual fixed costs, ζ_{var} the total variable costs accumulating over one year, ζ_{fuel} the accumulated fuel costs over one year and ζ_{env} the annual penalties for environmental pollution. These costs are then calculated in the following way:

Annualized invest costs

Investments are typically depreciated over a longer period of time than the standard modeling horizon of one year. To overcome distortions in the overall cost function urbs uses the annual cash flow (CAPEX) for the calculation of the investment costs in the cost function. This is captured by multiplying the total invest costs for a given process C_p with the so-called annuity factor f_p , i.e.:

$$\zeta_{\text{inv},p} = f_p \cdot C_p$$

For an interest rate of i and a depreciation period of n years the annuity factor can be derived using the remaining debt after k payments C_k :

$$\text{After 0 Payments: } C_0 = C(1 + i)$$

$$\text{After 1 Payment: } C_1 = (C_0 - fC)(1 + i) = C(1 + i)^2 - fC(1 + i)$$

$$\text{After 2 Payments: } C_2 = (C_1 - fC)(1 + i) = C(1 + i)^3 - fC(1 + i)^2 - fC(1 + i)$$

...

$$\text{After n Payments: } C_n = C(1 + i)^n + C \sum_{k=0}^{n-1} (1 + i)^k = (1 + i)^n + f \left(\frac{1 - (1 + i)^n}{i} \right).$$

Since the outstanding debt becomes 0 at the end of the depreciation period this leads to:

$$f = \frac{(1 + i)^n \cdot i}{(1 + i)^n - 1}$$

The annualized invest costs for all investments made by the optimizer are then given by:

$$\zeta_{\text{inv}} = \sum_{p \in P_{\text{exp}}} f_p k_p^{\text{inv}} \hat{\kappa}_p,$$

where k_p^{inv} signifies the specific invest costs of process p per unit capacity and P_{exp} is the subset of all processes that are actually expanded.

Annual fixed costs

The annual fixed costs represent maintenance and staff payments the processes used. They are playing a role for unit expansion only and are given as parameters for all allowed processes. Fixed costs scale with the capacity (in W) of the processes, and can be calculated using:

$$\zeta_{\text{fix}} = \sum_{p \in P} k_p^{\text{fix}} \kappa_p,$$

where k_p^{fix} represents the specific annual fix costs for process p .

Annual variable costs

Variable costs represent both, additional maintenance requirements due to usage of processes and taxes or tariffs. They scale with the utilization of processes (in Wh) and can be calculated in the following way:

$$\zeta_{\text{var}} = w \Delta t \sum_{t \in T_m} p \in P k_{pt}^{\text{var}} \tau_{pt},$$

where k_{pt}^{var} are the specific variable costs per time integrated process usage, and w and Δt are a weight factor that extrapolates the actual modeled time horizon to one year and the timestep length in hours, respectively.

Annual fuel costs

The usage of fuel adds an additional cost factor to the total costs. As with variable costs these costs occur when processes are used and are dependent on the total usage of the fuel (stock) commodities:

$$\zeta_{\text{fuel}} = w \Delta t \sum_{t \in T_m} c \in C_{\text{stock}} k_c^{\text{fuel}} \rho_c,$$

where k_c^{fuel} are the specific fuel costs. The distinction between variable and fuel costs is introduced for clarity of the results, both could in principle be merged into one class of costs.

Annual environmental costs

Environmental costs occur when the emission of an environmental commodity is penalized by a fine. Environmental commodities do not have to be balanced but can be emitted to the surrounding. The total production of the polluting environmental commodity is then given by:

$$\zeta_{\text{env}} = -w \Delta t \sum_{t \in T_m} c \in C_{\text{env}} k_c^{\text{env}} \text{CB}(c, t),$$

where k_c^{env} are the specific costs per unit of environmental commodity and CB is the momentary commodity balance of commodity c at time t . The minus sign is due to the sign convention used for the commodity balance which is positive when the system takes in a unit of a commodity.

After this discussion of the individual cost terms the constraints making up the matrices A and B are discussed now.

Process expansion constraints

The unit expansion constraints are independent of the modeled time. In case of the minimal model the are restricted to two constraints only limiting the allowed capacity expansion for each process. The total capacity of a given process is simply given by:

$$\begin{aligned} \forall p \in P : \\ \kappa_p &= K_p + \hat{\kappa}_p, \end{aligned}$$

where K_p is the already installed capacity of process p . The newly installed capacity can also be an integer, expressed as the product between the parameter process new capacity block K_p^{block} and the variable new process capacity units β_p :

$$\hat{\kappa}_p = K_p^{\text{block}} \cdot \beta_p$$

Process capacity limit rule

The capacity of each process p is limited by a maximal and minimal capacity, \overline{K}_p and \underline{K}_p , respectively, which are both given to the model as parameters:

$$\begin{aligned} \forall p \in P : \\ \underline{K}_p \leq \kappa_p \leq \overline{K}_p. \end{aligned}$$

All further constraints are time dependent and are determinants of the unit commitment, i.e. the time series of operation of all processes and commodity flows.

Commodity dispatch constraints

In this part the rules governing the commodity flow timeseries are shown.

Vertex rule (“Kirchhoffs current law”)

This rule is the central rule for the commodity flows and states that all commodity flows, (except for those of environmental commodities) have to be balanced in each time step. As a helper function the already mentioned commodity balance is calculated in the following way:

$$\begin{aligned} \forall c \in C, t \in T_m : \\ \text{CB}(c, t) = \sum_{(c,p) \in C_p^{\text{out}}} \epsilon_{cpt}^{\text{in}} - \sum_{(c,p) \in C_p^{\text{in}}} \epsilon_{cpt}^{\text{out}}. \end{aligned}$$

Here, the tuple sets $C_p^{\text{in,out}}$ represent all input and output commodities of process p , respectively. The commodity balance thus simply calculates how much more of commodity c is emitted by than added to the system via process p in timestep t . Using this term the vertex rule for the various commodity types can now be written in the following way:

$$\forall c \in C_{\text{st}}, t \in T_m : \rho_{ct} \geq \text{CB}(c, t),$$

where C_{st} is the set of stock commodities and:

$$\forall c \in C_{\text{dem}}, t \in T_m : -d_{ct} \geq \text{CB}(c, t),$$

where C_{dem} is the set of demand commodities and d_{ct} the corresponding demand for commodity c at time t . These two rules thus state that all stock commodities that are consumed at any time in any process must be taken from the stock and that all demands have to be fulfilled at each time step.

Stock commodity limitations

There are two rule that govern the retrieval of stock commodities from stock: The total stock and the stock per hour rule. The former limits the total amount of stock commodity that can be retrieved annually and the latter limits the same quantity per timestep. the two rules take the following form:

$$\begin{aligned} \forall c \in C_{\text{st}} : \\ w \sum_{t \in T_m} \rho_{ct} \leq \bar{L}_c \end{aligned}$$

$$\begin{aligned} \forall c \in C_{\text{st}}, t \in T_m : \\ \rho_{ct} \leq \bar{l}_c, \end{aligned}$$

where \bar{L}_c and \bar{l}_c are the totally allowed annual and hourly retrieval of commodity c from the stock, respectively.

Environmental commodity limitations

Similar to stock commodities, environmental commodities can also be limited per hour or per year. Both properties are assured by the following two rules:

$$\begin{aligned} \forall c \in C_{\text{env}} : \\ -w \sum_{t \in T_m} \text{CB}(c, t) \leq \bar{M}_c \end{aligned}$$

$$\begin{aligned} \forall c \in C_{\text{env}}, t \in T_m : \\ -\text{CB}(c, t) \leq \bar{m}_c, \end{aligned}$$

where \bar{M}_c and \bar{m}_c are the totally allowed annual and hourly emissions of environmental commodity c to the atmosphere, respectively.

Process dispatch constraints

So far, apart from the commodity balance function, the interaction between processes and commodities have not been discussed. It is perhaps in order to start with the general idea behind the modeling of the process operation. In urbs all processes are mimo-processes, i.e., in general they take in multiple commodities as inputs and give out multiple commodities as outputs. The respective ratios between the respective commodity flows remain normally fixed. The operational state of the process is then captured in just one variable, the process throughput τ_{pt} and is linked to the commodity flows via the following two rules:

$$\begin{aligned} \forall p \in P, c \in C, t \in T_m : \\ \epsilon_{pct}^{\text{in}} = r_{pc}^{\text{in}} \tau_{pt} \\ \epsilon_{pct}^{\text{out}} = r_{pc}^{\text{out}} \tau_{pt}, \end{aligned}$$

where $r_{pc}^{\text{in}, \text{out}}$ are the constant factors linking the commodity flow to the operational state. The efficiency η of the process p for the conversion of commodity c_1 into commodity c_2 is then simply given by:

$$\eta = \frac{r_{pc_2}^{\text{out}}}{r_{pc_1}^{\text{in}}}.$$

Basic process throughput rules

The throughput τ_{pt} of a process is limited by its installed capacity and the specified minimal operational state. Furthermore, the switching speed of a process can be limited:

$$\begin{aligned} \forall p \in P, t \in T_m : \\ \tau_{pt} &\leq \kappa_p \\ \tau_{pt} &\geq \underline{P}_p \kappa_p \\ \tau_{pt} - \tau_{p(t-1)} &\leq \Delta t \overline{PG}_p^{\text{up}} \kappa_p \\ \tau_{pt} - \tau_{p(t-1)} &\geq -\Delta t \overline{PG}_p^{\text{down}} \kappa_p \end{aligned}$$

where \underline{P}_p is the normalized, minimal operational state of the process and $\overline{PG}_p^{\text{up}}$ and $\overline{PG}_p^{\text{down}}$ are the normalized, maximal ramping up gradient, respectively ramping down gradient of the operational state in full capacity per timestep.

Intermittent supply rule

If the input commodity is of type ‘SupIm’, which means that it represents an operational state rather than a proper material flow, the operational state of the process is governed by this alone. This feature is typically used for renewable energies but can be used whenever a certain operation time series of a given process is desired

$$\begin{aligned} \forall p \in P, c \in C_{\text{sup}}, t \in T_m : \\ \epsilon_{cpt}^{\text{in}} &= s_{ct} \kappa_p. \end{aligned}$$

Here, s_{ct} is the time series that governs the exact operation of process p , leaving only its capacity κ_p as a free variable.

This concludes the minimal model.

Intertemporal optimization model

Intertemporal models are a more general type of model than the minimal case. For such models a second time domain is introduced to capture the behavior of the system over a timeframe of many years, thus rendering a modeling of the system development, rather than the optimal system configuration, possible. To keep the model as small as possible while still capturing most of the intertemporal behavior, the second time slice is approximated by a number of support timeframes (years) $Y = (y_1, \dots, y_n)$, which is in general smaller than the total model horizon. Each modeled timeframe is then essentially a minimal (or multinode-) model in its own right. The basic approximative assumptions linking the modeled timeframes are then given by:

- Each modeled year is repeated k times if the next modeled year is k years later. The last year is repeated a user specified number of times.
- The depreciation period is assumed to be also the operational period of any unit built. There is no operation in an economically fully depreciated state.
- A unit can only be operated in a given modeled year when it is operational for the entire period that year represents, i.e., until the next modeled year.

- All payments are exponentially discounted with a discount rate j that is set once for the entire modeling horizon.

The variable vector is as a first step only changed in so far, as the second time domain is entering the index. It now reads:

$$x^T = (\zeta, \underbrace{\rho_{yct}}_{\text{commodity variables}}, \underbrace{\kappa_{yp}, \hat{\kappa}_{yp}, \tau_{ypt}, \epsilon_{ycpt}^{\text{in}}, \epsilon_{ycpt}^{\text{out}}}_{\text{process variables}}).$$

Here, ζ represents the total discounted system costs over the entire modeling horizon, ρ_{yct} the amount of commodities c taken from a virtual, infinite stock in year y at time t , κ_{yp} and $\hat{\kappa}_{yp}$ the total and the newly installed process capacities in year y of processes p , τ_{ypt} the operational state in year y of processes p at time t and $\epsilon_{ycpt}^{\text{in}}$ and $\epsilon_{ycpt}^{\text{out}}$ the total inputs and outputs in year y of commodities c to and from process p at time t , respectively.

All dispatch constraint equations for commodities and processes described in the minimal model section, as well as all such constraints for transmissions, storages, DSM described in their respective dedicated sections, remain structurally the same in an intertemporal model. The only modification there is, that the modeled year shows up as an additional index.

The parts that change in a more meaningful way are the costs and the unit expansion constraints.

Costs

As in the minimal model the total cost variable can be split into the following sum:

$$\zeta = \zeta_{\text{inv}} + \zeta_{\text{fix}} + \zeta_{\text{var}} + \zeta_{\text{fuel}} + \zeta_{\text{env}},$$

where ζ_{inv} are the discounted invest costs accumulated over the entire modeled period, ζ_{fix} the discounted, accumulated fixed costs, ζ_{var} the discounted, sum over the modeled years of all variable costs accumulated over each year, ζ_{fuel} the discounted sum over the modeled years of fuel costs accumulated over each year and ζ_{env} the discounted total penalty for environmental pollution.

All costs are discounted by the same exponent j for the entire modeling horizon on a yearly basis. This means that any payment x that has to be made in a year k will be discounted for the cost function ζ by:

$$x_{\text{discounted}} = (1 + j)^{-k} \cdot x$$

Since all non-modeled years are just treated as exact copies of the last modeled year before them, the discounted sum of fix, variable, fuel and environmental costs can simply be taken as the costs of the representative modeled year m multiplied by a factor D_m . If the distance to the next modeled year is k , it can be calculated via:

$$\begin{aligned} D_m &= \sum_{l=m}^{m+k-1} (1 + j)^{-l} = (1 + j)^{-m} \sum_{l=0}^{k-1} (1 + j)^{-l} = (1 + j)^{-m} \frac{1 - (1 + j)^{-k}}{1 - (1 + j)^{-1}} = \\ &= (1 + j)^{1-m} \frac{1 - (1 + j)^{-k}}{j}. \end{aligned}$$

So for example the variable costs for modeled year m and its k identical, non-modeled copies $\zeta_{\text{var}}^{\{m, m+1, \dots, m+k-1\}}$ are given by:

$$\zeta_{\text{var}}^{\{m, m+1, \dots, m+k-1\}} = D_m \cdot \zeta_{\text{var}}^m,$$

if ζ_{var}^m is the sum of all variable costs accumulated by the use of units in the year m alone by the model.

Intertemporal calculation of invest costs

In the intertemporal model, invest costs are calculated using the annuity method. This directly entails that there are no rest values of any units built by the model that have to be considered for the cost function. It is then possible to multiply the annuity payments fC for a unit with investment costs C built in year m simply with the factor D_m . The only difference is, that the investment annuity payments are not restricted to the modeled years but have to be paid for the entire depreciation period provided that it is within the modeled time horizon. When the depreciation period is n and k is the number of payments that fall in the modeled time horizon, the total costs C_{total} of an investment of size C made in year m is given by:

$$\begin{aligned} C_m^{\text{total}} &= D_m \cdot f \cdot C = (1+j)^{1-m} \frac{1 - (1+j)^{-k}}{j} \cdot \frac{(1+i)^n \cdot i}{(1+i)^n - 1} \cdot C = \\ &= (1+j)^{1-m} \cdot \underbrace{\frac{i}{j} \cdot \left(\frac{1+i}{1+j}\right)^n \cdot \frac{(1+j)^n - (1+j)^{n-k}}{(1+i)^n - 1}}_{=: I_m} \cdot C \end{aligned}$$

For either $i = 0$ or $j = 0$ a distinction has to be made, which takes the following form:

- $i = 0, j = 0$:

$$C_m^{\text{total}} = \underbrace{\frac{k}{n}}_{=: I_m} \cdot C$$

- $i \neq 0, j = 0$:

$$C_m^{\text{total}} = k \cdot f \cdot C = k \cdot \underbrace{\frac{(1+i)^n \cdot i}{(1+i)^n - 1}}_{=: I_m} \cdot C$$

- $i = 0, j \neq 0$:

$$C_m^{\text{total}} = \frac{1}{n} \cdot (1+j)^{-m} \sum_{l=0}^{k-1} (1+j)^{-l} \cdot C = \underbrace{\frac{1}{n} \cdot (1+j)^{-m} \cdot \frac{(1+j)^k - 1}{(1+j)^k \cdot j}}_{=: I_m} \cdot C$$

In any case the total invest costs are then given by:

$$\begin{aligned} \zeta_{\text{inv}} &= \sum_{y \in Y} \\ p \in PC_m^{\text{total}} &= \sum_{y \in Y} \\ p &\in PI_y k_{yp}^{\text{inv}} \hat{\kappa}_{yp} \end{aligned}$$

Unit expansion constraints

Apart from the costs there are also changes in the unit expansion constraints for an intertemporal model. These changes mostly concern how the amount of installed units is found. This becomes an issue since

units built in an earlier modeled year or already installed in the first modeled year, may or may not be operational in a given modeled year m and through $m + k - 1$. Here, k is the distance to the next modeled year or the end of the modeled horizon in case of m being the last modeled year. To properly calculate the capacity of a process in a year y the following two sets are necessary:

$$O := \{(p, y_i, y_j) | p \in P, \{y_i, y_j\} \in Y, y_i \leq y_j, y_i + L_p \geq y_{j+1}\}$$

$$O_{\text{inst}} := \{(p, y_j) | p \in P_0, y \in Y, y_0 + T_p \geq y_{j+1}\},$$

where L_p is the lifetime of processes p , P_0 the subset of processes that are already installed in the first modeled year y_0 and T_p the rest lifetime of already installed processes. If y_j is the last modeled year, y_{j+1} stands for the end of the model horizon.

With these two sets the installed process capacity in a given year is then given by:

$$\kappa_{yp} = \sum_{y' \in Y} (p, y', y) \in O_{\text{inst}} \hat{\kappa}_{y'p} + K_p, \text{ if } (p, y) \in O_{\text{inst}}$$

$$\kappa_{yp} = \sum_{y' \in Y} (p, y', y) \in O_{\text{inst}} \hat{\kappa}_{y'p}, \text{ else}$$

where K_p is the installed capacity of process p at the beginning of the modeling horizon. Since for each modeled year still the capacity constraint

$$\forall y \in Y, p \in P : \\ \underline{K}_{yp} \leq \kappa_{yp} \leq \overline{K}_{yp}$$

is valid, the set constraints can have effects across years and especially the modeller has to be careful not to set infeasible constraints.

Commodity dispatch constraints

While in an intertemporal model all commodity constraints within one modeled year remain valid one addition is possible concerning CO2 emissions. Here, a budget can be given, which is valid over the entire modeling horizon:

$$-w \sum_{y \in Y} t \in T_m \text{CB}(y, \text{CO}_2, t) \leq \overline{\overline{L}}_{\text{CO}_2}$$

Here, $\overline{\overline{L}}_c$ is the global budget for the emission of the environmental commodity. Currently this is hard coded for CO2 only.

This rule concludes the model additions introduced by intertemporal modeling.

Multinode optimization model

The introduction of multiple spatial nodes into the model is the second big extension of the minimal model that is possible. Similar to the intertemporal model expansion it also adds an index level to

all variables and parameters. This addition is perpendicular to the intertemporal modeling and both extensions do not interact in any complex way with each other. Here, the multinode model extension will be shown without the intertemporal extension, i.e., it is shown as an extension to the minimal model. In this case the variable vector of the optimization problem reads:

$$x^T = (\zeta, \underbrace{\rho_{vct}}_{\text{commodity variables}}, \underbrace{\kappa_{vp}, \hat{\kappa}_{vp}, \tau_{vpt}, \epsilon_{vcpt}^{\text{in}}, \epsilon_{vcpt}^{\text{out}}}_{\text{process variables}}, \underbrace{\kappa_{af}, \hat{\kappa}_{af}, \pi_{aft}^{\text{in}}, \pi_{aft}^{\text{out}}}_{\text{transmission variables}}).$$

Here, ζ represents the total annualized system cost across all modeled vertices $v \in V$, ρ_{vct} the amount of commodities c taken from a virtual, infinite stock at vertex v and time t , κ_{vp} and $\hat{\kappa}_{vp}$ the total and the newly installed process capacities of processes p at vertex v , τ_{vpt} the operational state of processes p at vertex v and time t , $\epsilon_{vcpt}^{\text{in}}$ and $\epsilon_{vcpt}^{\text{out}}$ the total inputs and outputs of commodities c to and from process p at vertex v and time t , κ_{af} and $\hat{\kappa}_{af}$ the installed and new capacities of a transmission line f linking two vertices with the arc a and π_{aft}^{in} and π_{aft}^{out} the in- and outflows into arc a via transmission line f at time t .

There are no qualitative changes to the cost function only the sum of all units now extends over processes and transmission lines.

Transmission capacity constraints

Transmission lines are modeled as unidirectional arcs in urbs. This means that they have a input site and an output site. Furthermore, an arc already specifies a commodity that can travel across it. However, from the modelers point of view the transmissions rather behave like non-directional edges, linking both sites with the identical capacity in both directions. This behavior is then ensured by the transmission symmetry rule, which sets the capacity of both unidirectional arcs to be identical:

$$\begin{aligned} \forall a \in V \times V \times C, f \in F : \\ \kappa_{af} = \kappa_{a'f}, \end{aligned}$$

where a' is the inverse arc of a . The transmission capacity is then calculated similar to process capacities in the minimal model:

$$\begin{aligned} \forall a \in V \times V \times C, f \in F : \\ \kappa_{af} = K_{af} + \hat{\kappa}_{af}, \end{aligned}$$

where K_{af} represents the already installed and $\hat{\kappa}_{af}$ the new capacity of transmission f installed in arc a . The new capacity can also be expressed as the product of the parameter transmission capacity block K_{yaf}^{block} and the variable new transmission capacity units β_{yaf} :

$$\hat{\kappa}_{af} = K_{yaf}^{\text{block}} \cdot \beta_{yaf}$$

Transmission capacity limit rule

Completely analogous to processes also transmission line capacities are limited by a maximal and minimal allowed capacity \bar{K}_{af} and \underline{K}_{af} via:

$$\begin{aligned} \forall a \in V \times V \times C, f \in F : \\ \underline{K}_{af} \leq \kappa_{af} \leq \bar{K}_{af} \end{aligned}$$

Commodity dispatch constraints

Apart from these time independent rules, the time dependent rules governing the unit utilization are amended with respect to the minimal model by the introduction of transmission lines.

Amendments to the Vertex rule

The vertex rule is changed, since additional commodity flows through the transmission lines occur in each vertex. The commodity balance function is thus changed to:

$$\forall c \in C, t \in T_m :$$

$$\text{CB}(c, t) = \sum_{(c,p) \in C_p^{\text{in}}} \epsilon_{vcpt}^{\text{in}} + \sum_{(a,f) \in A_v^{\text{in}}} \pi_{aft}^{\text{in}} - \sum_{(c,p) \in C_p^{\text{out}}} \epsilon_{vcpt}^{\text{out}} - \sum_{(a,f) \in A_v^{\text{out}}} \pi_{aft}^{\text{out}}.$$

Here, the new tuple sets $A_v^{\text{in,out}}$ represent all input and output arcs a connecting vertex v , respectively. The commodity balance is thereby allowing for commodities to leave the system at vertex v via arcs as well as processes. Apart from this change to the commodity balance the vertex rule and the other rules restricting commodity flows remain unchanged with respect to the minimal model.

Global CO2 limit

In addition to the general vertex specific constraint for the emissions of environmental commodities as discussed in the minimal model, there is a hard coded possibility to limit the CO2 emissions across all modeled sites:

$$t \in T_m \text{CB}(v, \text{CO}_2, t) \leq \bar{L}_{\text{CO}_2, y} - w \sum_{v \in V}$$

Transmission dispatch constraints

There are two main constraints for the commodity flows to and from transmission lines. The first restricts the total amount of commodity c flowing in arc a on transmission line f to the total capacity of the line:

$$\forall a \in V \times V \times C, f \in F, t \in T_m : \\ \pi_{aft}^{\text{in}} \leq \kappa_{af}.$$

Here, the input into the arc π_{aft}^{in} is taken as a reference for the total capacity. The output of the arc in the target site is then linked to the input with the transmission efficiency e_{af}

$$\forall a \in V \times V \times C, f \in F, t \in T_m : \\ \pi_{aft}^{\text{out}} = e_{af} \cdot \pi_{aft}^{\text{in}}.$$

DC Power Flow feature

Transmission lines can be modelled with DC Power Flow as an optional feature to represent the AC network grid. With the DC Power Flow feature, the variable voltage angle is introduced for the vertices connected with DC Power Flow transmission lines. The DC Power Flow is defined by the relation between the voltage angle θ_{vt} of connecting vertices.

It is possible to combine the default transmission model with the DC Power Flow transmission model. The DCPF feature can be activated on the selected transmission lines. This way two different sets of transmission tuples, subject to different constraints, will be modelled. These transmission tuple sets are defined as the set of transport model (default) transmission lines $F_{cv_{\text{out}}v_{\text{in}}}^{TP}$ and the set of DCPF transmission lines $F_{cv_{\text{out}}v_{\text{in}}}^{DCPF}$.

Usage

This feature can be activated for selected transmission lines by including the following parameters:

- The reactance X_{af} of a transmission line is required to be included in the model input to model the given transmission line with DCPF. This parameter should be greater than 0 and given in per-unit system. If this parameter is excluded from the model input, DCPF will not be activated for the transmission line.
- The voltage angle difference of two connecting sites should be limited with angle difference limit \overline{dl}_{af} to create a stable model. This parameter is required to limit the voltage angle difference between two connecting sites. A degree value between 0 and 91 is allowed.
- The base voltage $V_{af\text{base}}$ of transmission lines are required to convert the power flow from per-unit system to MW. The base voltage parameter is required in kV for every transmission line, which should be modelled with DCPF. The value of this parameter should be greater than 0.
- Since the DC Power Flow model ignores the loss of a transmission line, the efficiency e_{af} of the transmission lines modelled with the DCPF should be set to 100% represented with the value “1”.

Contrary to the default transmission line representation, DC Power Flow transmission lines are represented with a single bidirectional arc between two vertices. The complementary arc of a DC Power Flow transmission line will be excluded from the model even if it is defined by the user. Depending on the voltage angle difference of two connecting sites, the power flow π_{aft} on a DC Power Flow transmission line can be both negative or positive indicating the direction of the flow.

DC Power Flow Equation

Power flow on a transmission line modelled with DCPF:

$$\pi_{aft}^{\text{in}} = \frac{(\theta_{v_{\text{int}}} - \theta_{v_{\text{out}}})}{57.2958} \left(-\frac{1}{X_{af}}\right) V_{af\text{base}}^2$$

Here $\theta_{v_{\text{int}}}$ and $\theta_{v_{\text{out}}}$ are the voltage angles of the source site v_{in} and destination site v_{out} . These are converted to radian from degrees by dividing by 57,2958. X_{af} is the reactance of the transmission line in per unit system and $\left(-\frac{1}{X_{af}}\right)$ is the admittance of the transmission line.

Constraints

Constraints applied to the DCPF transmission lines vary from those applied to the transport transmission lines.

Symmetry rule is ignored for the DCPF transmission lines, since these lines only consist of single bidirectional arcs. Since the DCPF transmission lines do not have complementary arcs the fixed and investment costs would be halved. To prevent this error caused by the excluded symmetry constraint for DCPF transmission lines, fixed and investment prices for DCPF lines are doubled automatically before calculating the costs.

The constraint which restricts the commodity flow π_{aft}^{in} on a transmission line with the installed capacity κ_{af} is expanded for DCPF transmission lines. The additional constraint restricts the lower limit of the power flow, since the power flow with DCPF can also be negative.

$$-\pi_{aft}^{\text{in}} \leq \kappa_{af}$$

Voltage angle difference of two connecting vertices v_{in} and v_{out} is restricted with the angle difference limit parameter \overline{dl}_{af} given for a DCPF transmission f on an arc a

$$-\overline{dl}_{af} \leq (\theta_{v_{in}t} - \theta_{v_{out}t}) \leq \overline{dl}_{af}$$

Two additional constraints are used in DCPF feature to retrieve the absolute value $\pi_{aft}^{in'}$ of the power flow on a DCPF transmission line, which is included in the variable cost calculation. With the help of these constraints and minimization of objective function, which includes the substitute variable $\pi_{aft}^{in'}$, the substitute variable will be equal to the absolute value of the power flow variable $|\pi_{aft}^{in}|$

$$\pi_{aft}^{in'} \geq \pi_{aft}^{in}$$

$$\pi_{aft}^{in'} \geq -\pi_{aft}^{in}$$

Energy Storage

Storages can optionally be set in urbs. They introduce additional variables and constraints, contribute to the cost function but do not increase the index depth of all variables and parameters. For this and all the further features all variables will be written in the full index depth, i.e. for intertemporal models with multiple vertices. For storages the capacity and the charging/discharging power are expanded independently. For each storage one commodity is specified which is stored. It is thus not necessary to specify the commodity as an extra index in the variables and parameters. With added storages the variable vector then reads:

$$x^T = (\zeta, \underbrace{\rho_{yvct}}_{\text{commodity variables}}, \underbrace{\kappa_{yvp}, \widehat{\kappa}_{yvp}, \tau_{yvpt}, \epsilon_{yvcpt}^{in}, \epsilon_{yvcpt}^{out}}_{\text{process variables}}, \underbrace{\kappa_{yaf}, \widehat{\kappa}_{yaf}, \pi_{yaf}^{in}, \pi_{yaf}^{out}}_{\text{transmission variables}}, \underbrace{\kappa_{yvs}^c, \kappa_{yvs}^p, \widehat{\kappa}_{yvs}^c, \widehat{\kappa}_{yvs}^p, \epsilon_{yvst}^{in}, \epsilon_{yvst}^{out}, \epsilon_{yvst}^{con}}_{\text{storage variables}}).$$

Here, the new storage variables $\kappa_{yvs}^{c,p}$ and $\widehat{\kappa}_{yvs}^{c,p}$ stand for the total and new capacities of storage capacity and power of storage unit s , in modeled year y at vertex v , respectively, the variables $\epsilon_{yvst}^{in,out}$ represent the input and output to storage s in year y at vertex v at time t and ϵ_{yvst}^{con} the storage state.

Costs

The costs are changed in a straightforward way. The invest, fix and variable costs are now summed over the storage capacities, powers and the total amount of charged and discharged commodity in addition to the process indices. As in the case of transmissions there are no qualitative changes to the costs.

Storage expansion constraints

Storages are expanded in their capacity and charging and discharging power separately. The respective constraints read:

$$\kappa_{yvs}^{c,p} = \sum_{y' \in Y} \kappa_{y'vs}^{c,p}$$

$$(s, v, y', y) \in O_{\hat{\kappa}_{y'vs}^{c,p}} + K_{vs}, \text{ if } (s, v, y) \in O_{\text{inst}}$$

$$\kappa_{yvs}^{c,p} = \sum_{y' \in Y} \hat{\kappa}_{y'vs}^{c,p}$$

$$(s, v, y', y) \in O_{\hat{\kappa}_{y'vs}^{c,p}}, \text{ else,}$$

where $\kappa_{yvs}^{c,p}$ are the total installed capacity and power, respectively, in year y at site v of storage s and $\hat{\kappa}_{yvs}^{c,p}$ the corresponding

newly installed storage capacities and powers. Both newly installed quantities can also be expressed as the product of the parameter storage new capacity/power block $K_{yvs}^{c,p \text{ block}}$ and the variable new storage size/power units $\beta_{yvs}^{c,p}$:

$$\hat{\kappa}_{yvs}^{c,p} = K_{yvs}^{c,p \text{ block}} \cdot \beta_{yvs}^{c,p}$$

Both total installed quantities are then also given an upper and a lower bond via:

$$\forall y \in Y, v \in V, s \in S :$$

$$\underline{K}_{yvs}^c \leq \kappa_{yvs}^c \leq \overline{K}_{yvs}^c$$

$$\underline{K}_{yvs}^p \leq \kappa_{yvs}^p \leq \overline{K}_{yvs}^p$$

Commodity dispatch constraints

The commodity unit utilization constraints are expanded by the use of storages.

Amendments to the Vertex rule

The vertex rule is changed, since additional commodity flows into and out of the storages can occur. The commodity balance function is thus changed to:

$$\forall y \in Y, v \in V, c \in C, t \in T_m :$$

$$\text{CB}(y, v, c, t) = \sum_{(y,v,c,p) \in C_{y,v,c,p}^{\text{in}}} \epsilon_{vcpt}^{\text{in}} + \sum_{(y,v,s,c) \in C_{y,v,s,c}} \epsilon_{yfst}^{\text{in}} + \sum_{(y,a,f) \in A_v^{\text{in}}} \pi_{aft}^{\text{in}} -$$

$$- \sum_{(y,v,c,p) \in C_p^{\text{out}}} \epsilon_{vcpt}^{\text{out}} - \sum_{(y,v,s,c) \in C_{y,v,s,c}} \epsilon_{yfst}^{\text{out}} - \sum_{(y,a,f) \in A_v^{\text{out}}} \pi_{aft}^{\text{out}}.$$

Here, the new tuple sets $C_{y,v,s,c}^{\text{in,out}}$ represent all inputs and outputs in year y at vertex v of commodity c into storage s . The variables $\epsilon_{yfst}^{\text{in,out}}$ are then the inputs and outputs of commodities to and from storages.

Storage dispatch constraints

In a storage the energy content $\epsilon_{yvs}^{\text{con}}$ has to be calculated. This is achieved by simply adding all inputs to and subtracting all outputs from the storage content at the previous time step $\epsilon_{yvs(t-1)}^{\text{con}}$:

$$\forall y \in Y, v \in V, s \in S, t \in T_m :$$

$$\epsilon_{yvs}^{\text{con}} = \epsilon_{yvs(t-1)}^{\text{con}} \cdot (1 - d_{yvs})^{\Delta t} + e_{yvs}^{\text{in}} \cdot \epsilon_{yvs}^{\text{in}} - \frac{\epsilon_{yvs}^{\text{out}}}{e_{yvs}^{\text{out}}}.$$

Here, $e_{yvs}^{\text{in,out}}$ are the efficiencies for charging and discharging, respectively, and d_{yvs} is the hourly self discharge rate.

Basic storage dispatch rules

Similar to processes and transmission lines, inputs and outputs are limited by the power capacity of the storage:

$$\forall y \in Y, v \in V, s \in S, t \in T_m :$$

$$\epsilon_{yvs}^{\text{in,out}} \leq \Delta t \cdot \kappa_{yvs}^{\text{p}}.$$

Additionally, the storage content is limited by the total storage energy capacity:

$$\forall y \in Y, v \in V, s \in S, t \in T_m :$$

$$\epsilon_{yvs}^{\text{con}} \leq \kappa_{yvs}^{\text{c}}.$$

Initial and final state

In order to avoid windfall profits for the optimization by, e.g., emptying a storage over the model horizon, the initial and final storage content are linked via:

$$\forall y \in Y, v \in V, s \in S :$$

$$\epsilon_{yvs(t_1)}^{\text{con}} \leq \epsilon_{yvs(t_N)}^{\text{con}},$$

where $t_{1,N}$ are the initial and final modeled timesteps, respectively. The inequality simplifies the model solving by relaying an otherwise unnecessarily strict constraint. A small disadvantage arises when the system can gain costs or save CO2 by filling a storage. This case is, however, not too common. It is additionally possible for the user to fix the initial storage content via:

$$\forall y \in Y, v \in V, s \in S :$$

$$\epsilon_{yvs(t_1)}^{\text{con}} = \kappa_{yvs}^{\text{c}} I_{yvs},$$

where I_{yvs} is the fraction of the total storage capacity that is filled at the beginning of the modeling period.

Fixed energy/power ratio

It is sometimes desirable to fix the ratio between energy capacity and charging/discharging power for a given storage. This is modeled by the possibility to set a linear dependence between the capacities through a user-defined “energy to power ratio” $k_{yvs}^{\text{E/P}}$. Note that this constraint is only active for the

storages with a positive value under the column “ep-ratio” in the input file, and when this value is not given, the power and energy capacities can be sized independently

$$\forall y \in Y, v \in V, s \in S : \\ \kappa_{yvs}^c = \kappa_{yvs}^p k_{yvs}^{E/P}.$$

This concludes the storage feature.

Trading with an external market

In urbs it is possible to model the trade with an external market. For this two new commodity types, buy and sell commodities, are introduced. For each a time series representing the momentary cost at each timestep is given. This time series is of course known to the model in advance, which has two implications. First, the modeled system is considered too small to influence the external market and any possible influence is not captured by the model, and, second, the perfect price foresight can distort the results when compared to a realistic trader in a market. For models with buy and sell commodities the variable vector takes the following form:

$$x^T = (\underbrace{\zeta, \rho_{yvct}, \varrho_{yvct}, \psi_{yvct}}_{\text{commodity variables}}, \underbrace{\kappa_{yvp}, \hat{\kappa}_{yvp}, \tau_{yvpt}, \epsilon_{yvcpt}^{\text{in}}, \epsilon_{yvcpt}^{\text{out}}}_{\text{process variables}}, \underbrace{\kappa_{yaf}, \hat{\kappa}_{yaf}, \pi_{yaf}^{\text{in}}, \pi_{yaf}^{\text{out}}}_{\text{transmission variables}}),$$

where ϱ_{yvct} is the amount of sell commodity c sold to the external market in year y from vertex v at time t and ψ_{yvct} is the amount of buy commodity c bought from the external market in year y at vertex v and time t .

Costs

The cost function is amended by two new cost types when the trading with an external market is modeled, the purchase and the revenue costs

$$\zeta = \zeta_{\text{inv}} + \zeta_{\text{fix}} + \zeta_{\text{var}} + \zeta_{\text{fuel}} + \zeta_{\text{rev}} + \zeta_{\text{pur}} + \zeta_{\text{env}}.$$

The two new cost types are then specified by the following equations:

$$\begin{aligned} \zeta_{\text{rev}} &= -w\Delta t \sum_{y \in Y} \\ &v \in V \\ &c \in C_{\text{sell}} \\ &t \in T_m D_m \cdot k_{yvct}^{\text{bs}} \cdot \varrho_{yvct} \\ \\ \zeta_{\text{pur}} &= w\Delta t \sum_{y \in Y} \\ &v \in V \\ &c \in C_{\text{buy}} \\ &t \in T_m D_m \cdot k_{yvct}^{\text{bs}} \cdot \psi_{yvct}, \end{aligned}$$

where k_{yvct}^{bs} represents the time series of the given buy and sell commodity prices.

Commodity dispatch constraints

Buy and sell commodities change the vertex rule (Kirchhoff's current law), by adding a new way for in- and output flows of commodities. The rule is thus amended by the following two equations:

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{sell}}, t \in T_m : \\ -\varrho_{ct} \geq \text{CB}(c, t) \end{aligned}$$

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{buy}}, t \in T_m : \\ \psi_{ct} \geq \text{CB}(c, t). \end{aligned}$$

The commodity balance itself is not changed. The new rules state that any amount of energy sold needs to be provided to (negative CB) the system via processes, storages or transmission lines, while buy commodity consumed by processes, storages or transmission lines in the system has to be replenished.

Buy/sell commodity limitations

The trade with the market in each modeled year and each vertex can be limited per time step and for an entire year. This introduces the following constraints:

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{sell}} : \\ w \sum_{t \in T_m} \varrho_{ct} \leq \bar{G}_{yvc} \end{aligned}$$

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{sell}}, t \in T_m : \\ \varrho_{yvct} \leq \bar{g}_{yvc} \end{aligned}$$

and

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{buy}} : \\ w \sum_{t \in T_m} \psi_{ct} \leq \bar{B}_{yvc} \end{aligned}$$

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{buy}}, t \in T_m : \\ \varrho_{yvct} \leq \bar{b}_{yvc}. \end{aligned}$$

Here, the parameters \bar{b}_{yvc} and \bar{B}_{yvc} limit the hourly and yearly maximums of buy from and \bar{g}_{yvc} and \bar{G}_{yvc} the hourly and yearly maximum of selling to the external market.

This concludes the discussion of the modeled trading with an external market.

Demand side management

Demand side management allows for the shifting of demands in time. It thus gives the model the possibility to divert from the strict restriction that all demands have to be fulfilled at all timesteps. Demand side management adds two variables to an urbs problem and the variable vector then reads:

$$x^T = (\zeta, \underbrace{\rho_{yvct}}_{\text{commodity variables}}, \underbrace{\kappa_{yvp}, \hat{\kappa}_{yvp}, \tau_{yvpt}, \epsilon_{yvcpt}^{\text{in}}, \epsilon_{yvcpt}^{\text{out}}}_{\text{process variables}}, \underbrace{\kappa_{yaf}, \hat{\kappa}_{yaf}, \pi_{yaf}^{\text{in}}, \pi_{yaf}^{\text{out}}}_{\text{transmission variables}}, \underbrace{\delta_{yvct}^{\text{up}}, \delta_{yvct}^{\text{down}}}_{\text{DSM variables}}).$$

The new variable $\delta_{yuct}^{\text{up}}$ represent the upshift of the momentary demand at time t and $\delta_{yuct(tt)}^{\text{down}}$ the corresponding downshifts. The downshifts need two time indices as they are referencing to the corresponding upshift with the first index t and the timesteps they actually occur via the second time index tt . The latter is then restricted to an interval around the reference upshift since loads cannot in general be shifted indefinitely. As it is modeled in urbs, DSM does not introduce any costs. To clarify the terms used for the DSM feature the following illustrative example is helpful.

Example of a DSM process

An example scenario with parameters below can be used to clarify the mathematical structure of a DSM process.

Site	Commodity	delay	eff	recov	cap-max-do	cap-max-up
South	Elec	3	1	1	2000	2000

First, an series of three upshifts, i.e. demand increases, indexed with the modeled timesteps 3,4 and 5 occurs in the example.

Table 1: DSM upshift process

t	
1	0
2	0
3	1445
4	1580
5	2000
6	0

The corresponding downshifts can then be visualized using a matrix, where the row index t corresponds to the upshifts above, that have to be compensated by downshifts. The modeled timesteps where the downshifts actually occur are labeled by tt and represent the column indices.

Table 2: DSM downshift process

$t \setminus tt$	1	2	3	4	5	6
1	0	0	0	0		
2	0	0	0	0	0	
3	1445	0	0	0	0	0
4	555	0	555	0	0	470
5		2000	0	0	0	0
6			0	0	0	0

The DSM upshift process is relatively easy to understand, for every time step t one upshift is made and it can not exceed 2000. The table for DSM downshift process shows, that the sum over all elements for every row index t , is equal to the upshift made at time step t . The blank spaces in the table are because of delay time restriction. For instance, an upshift in $t = 1$ may not be compensated with a downshift in $tt = 5$, as delay time is equal to 3 in our example. The restriction of the total DSM downshifts is given by the sum of all column elements for every index tt . This sum may not exceed 2000 as well, due to given parameters.

Commodity dispatch constraints

Demand side management changes the vertex rule. Every upshift δ_{yvc}^{up} leads to an additional demand, i.e., to an additional required output of the system, and vice versa for the downshifts. Effectively this changes the vertex rule (Kirchhoff's current law) for demand commodities with DSM to:

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{dem}}, t \in T_m : \\ -d_{yvc} - \delta_{yvc}^{\text{up}} &\geq \text{CB}(y, v, c, t) \\ -d_{yvc} + \sum_{tt \in [t-y_{yvc}, t+y_{yvc}]} \delta_{yvc(tt)}^{\text{down}} &\geq \text{CB}(y, v, c, t). \end{aligned}$$

The downshift equation requires a little elaboration. Here, the total downshift occurring at a timestep t can be caused by downshifts linked to different upshifts, which in the notation above occur at times tt . All downshift contributions within the delay time y_{yvc} of their respective upshifts are then summed up.

DSM variables rule

This central constraint rule for DSM in urbs links the up- and down shifts of DSM events. An upshift (multiplied with the DSM efficiency) at time t must be compensated with multiple downshifts during a certain time interval. The lower and upper bounds of this time interval are given by $t - y_{yvc}$ and $t + y_{yvc}$, where y_{yvc} is the delay time parameter specifying the allowed duration of a DSM event. Inside this time interval, another time index tt is required. It is used to index the downshift processes that are always linked to one upshift. Of course, the intervals of several upshifts can overlap. Mathematically, this rule can be noted like this:

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{dem}}^{\text{DSM}}, t \in T_m : \\ e_{yvc} \delta_{yvc}^{\text{up}} = \sum_{tt \in [t-y_{yvc}, t+y_{yvc}]} \delta_{yvc(tt)}^{\text{down}}, \end{aligned}$$

where e_{yvc} is the DSM efficiency. Note here, that the summation is over the timesteps where the downshifts are occurring as opposed to the vertex rule above, where the summation is over the timesteps of the corresponding upshifts.

DSM shift limitations

DSM shifts are limited in size in both directions. This is modeled by

$$\begin{aligned} \forall y \in Y, v \in V, c \in C_{\text{dem}}^{\text{DSM}}, t \in T_m : \\ \delta_{yvc}^{\text{up}} \leq \overline{K}_{yvc}^{\text{up}} \\ \sum_{tt \in [t-y_{yvc}, t+y_{yvc}]} \delta_{yvc(tt)}^{\text{down}} \leq \overline{K}_{yvc}^{\text{down}}, \end{aligned}$$

where again the downshifts are summed over the corresponding upshifts, making sure that at no time there is a total downshift sum larger than the set maximum value.

In addition to these limitations on the single shift directions, the total sum of shifts is also limited in an urbs model via:

$$\forall y \in Y, v \in V, c \in C_{\text{dem}}^{\text{DSM}}, t \in T_m :$$

$$\delta_{yvc}^{\text{up}} + \sum_{tt \in [t - y_{yvc}, t + y_{yvc}]} \delta_{yvc(tt)}^{\text{down}} \leq \max\{\bar{K}_{yvc}^{\text{up}}, \bar{K}_{yvc}^{\text{down}}\}.$$

DSM recovery

Assuming that DSM is linked to some real physical devices, it is necessary to allow these devices to have some minimal time between DSM events, where, e.g., the ability to perform DSM is recovered. This is modeled in the following way:

$$\forall y \in Y, v \in V, c \in C_{\text{dem}}^{\text{DSM}}, t \in T_m :$$

$$\sum_{tt=t}^{o_{yvc}/\Delta t - 1} \delta_{yvc(tt)}^{\text{up}} \leq \bar{K}_{yvc}^{\text{up}} \cdot y_{yvc},$$

where o_{yvc} is the recovery time in hours. This constraint limits the total amount of upshifted energy within the recovery period (lhs) to the maximum allowed energy shift retained for the maximum amount of allowed shifting time for one shifting event. This means that only one full shifting event can occur within the recovery period.

This concludes the demand side management constraints.

Advanced Processes

Several processes have a complicated, non-linear behavior. Those that can be modelled in urbs are explained here. These are: Time Variable Efficiency, Minimum Load and Part Load Behaviors and On/Off Behavior.

Time Variable Efficiency

It is possible to exogenously manipulate the output of a process by introducing a time series, which changes the output ratios and thus the efficiency of a given process in each given timestep. This introduces an additional set of constraints in the form:

$$\forall p \in P^{\text{TimeVarEff}}, c \in C - C^{\text{env}}, t \in T_m :$$

$$\epsilon_{ypct}^{\text{out}} = r_{ypc}^{\text{out}} f_{ypt}^{\text{out}} \tau_{ypct}.$$

Here, f_{pt}^{out} represents the normalized time series of the varying output ratio. This feature can be helpful when modeling, e.g., temperature dependent effects or maintenance intervals. Environmental commodities are intentionally excluded from the output manipulation. The reason for this is that they are typically directly linked to inputs as, e.g., CO2 emissions are linked to the fossil inputs. A manipulation of the output for environmental commodities would thus violate the mass balance of carbon in this case (e.g. coal).

When the process in question is a process with part load behavior the equation for the time variable efficiency case takes the following form:

$$\forall p \in P^{\text{part load}} \text{ and } p \in P^{\text{TimeVarEff}}, c \in C, t \in T_m :$$

$$\epsilon_{ypct}^{\text{out}} = \Delta t \cdot f_{ypt}^{\text{out}} \cdot \left(\frac{r_{ypc}^{\text{out}} - r_{ypc}^{\text{out}}}{1 - \underline{P}_{yp}} \cdot \underline{P}_{yp} \cdot \kappa_{yp} + \frac{r_{ypc}^{\text{out}} - \underline{P}_p r_{ypc}^{\text{out}}}{1 - \underline{P}_{yp}} \cdot \tau_{ypt} \right).$$

Minimum Load and Part Load Behaviors

There are some processes which theoretically can be turned on and off, while others typically operate as must-run units (e.g. nuclear power plants, heat-producing plants during the cold season etc.). These processes can either have a constant and load independent efficiency or a part-load behavior.

In the case of a minimum load behavior with a constant, load independent efficiency, the values of the input and of the output of a process remain unchanged when compared except for the fact that their values, together with the value of the throughput, stay between the following boundaries:

$$\forall p \in P^{\text{minimum load}}, c \in C, t \in T_m :$$

$$\underline{P}_p \cdot \kappa_p \cdot r^{\text{in,out}} \leq \epsilon_{pct}^{\text{in,out}} \leq \kappa_p \cdot r^{\text{in,out}},$$

$$\forall p \in P^{\text{part load}}, c \in C, t \in T_m :$$

$$\underline{P}_p \cdot \kappa_p \cdot \underline{r}^{\text{in,out}} \leq \epsilon_{pct}^{\text{in,out}} \leq \kappa_p \cdot r^{\text{in,out}},$$

where \underline{P}_p is the minimum load fraction, κ_p the installed capacity, $r^{\text{in,out}}$ the input/output ratios and $\underline{r}^{\text{in,out}}$ the minimum input/output ratios.


Many processes show a non-trivial part-load behavior. In particular, often a nonlinear reaction of the efficiency on the operational state is given. Although urbs itself is a linear program this can with some caveats be captured in many cases. The reason for this is, that the efficiency of a process is itself not given as a parameter, but is merely the ratio between input and output multipliers. It is thus possible to use purely linear functions to get a nonlinear behavior of the efficiency of the form:

$$\eta = \frac{a + b\tau_{pt}}{c + d\tau_{pt}},$$

where a,b,c and d are some constants. Specifically, the input and output ratios can be set to vary linearly between their respective values at full load $r_{pc}^{\text{in,out}}$ and their values at the minimal allowed operational state $\underline{P}_p \kappa_p$, which are given by $\underline{r}_{pc}^{\text{in,out}}$. This is achieved with the following equations and exemplified with the following graphic:

$$\forall p \in P^{\text{part load}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{in,out}} = \Delta t \cdot \left(\frac{r_{pc}^{\text{in,out}} - r_{pc}^{\text{in,out}}}{1 - \underline{P}_p} \cdot \underline{P}_p \cdot \kappa_p + \frac{r_{pc}^{\text{in,out}} - \underline{P}_p r_{pc}^{\text{in,out}}}{1 - \underline{P}_p} \cdot \tau_{pt} \right).$$

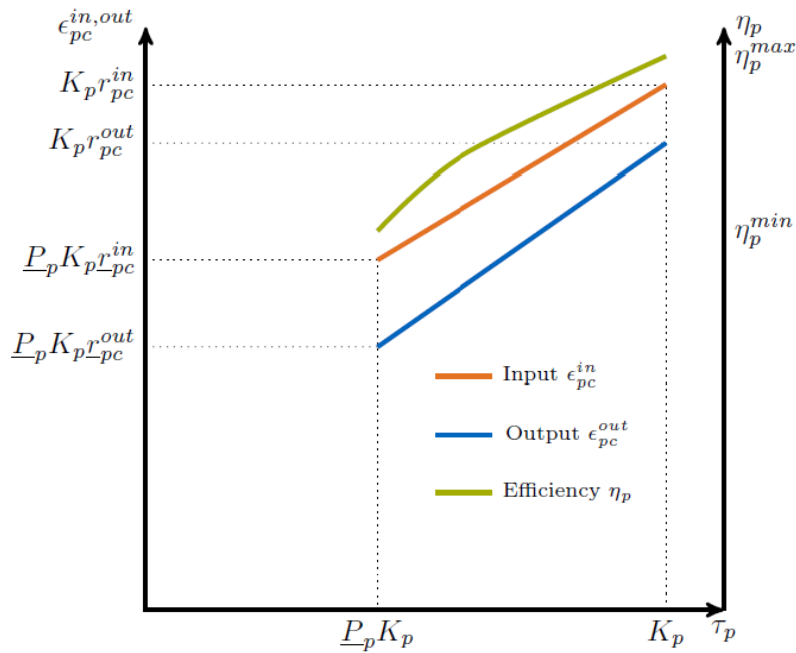


A few restrictions have to be kept in mind when using this feature:


- \underline{P}_p has to be set larger than 0 otherwise the feature will work but not have any effect.
- Environmental output commodities have to mimic the behavior of the inputs by which they are generated. Otherwise the emissions per unit of input would change together with the efficiency, which is typically not the desired behavior.

On/off Behavior

Some processes are characterised by a minimum or part-load behavior but still retain the practical necessity of being turned on and off if this is optimal. This feature transforms urbs from a linear problem to a quadratic integer problem, or piecewise linear. The following graphic illustrates a process with the on/off feature and constant efficiency:

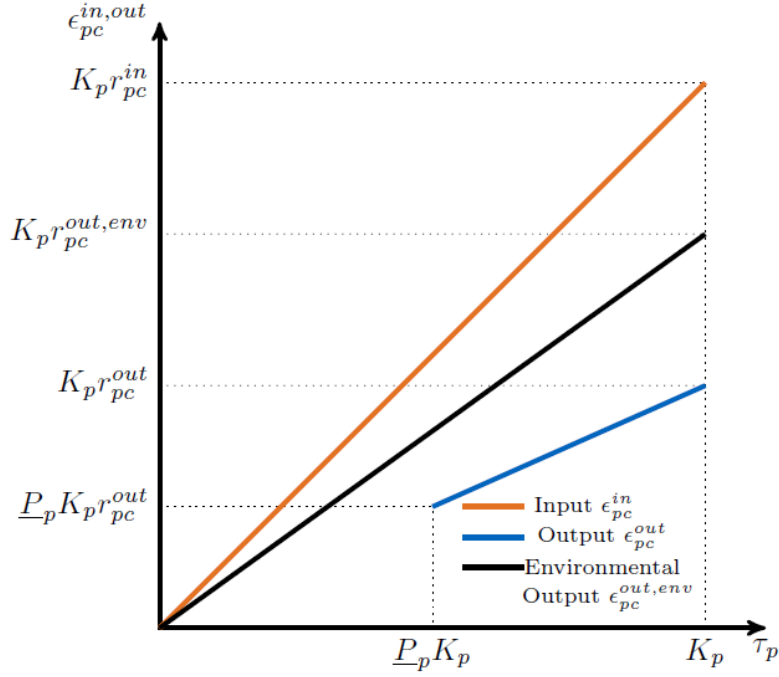

The following graphic illustrates a process with the on/off feature and part load behavior:

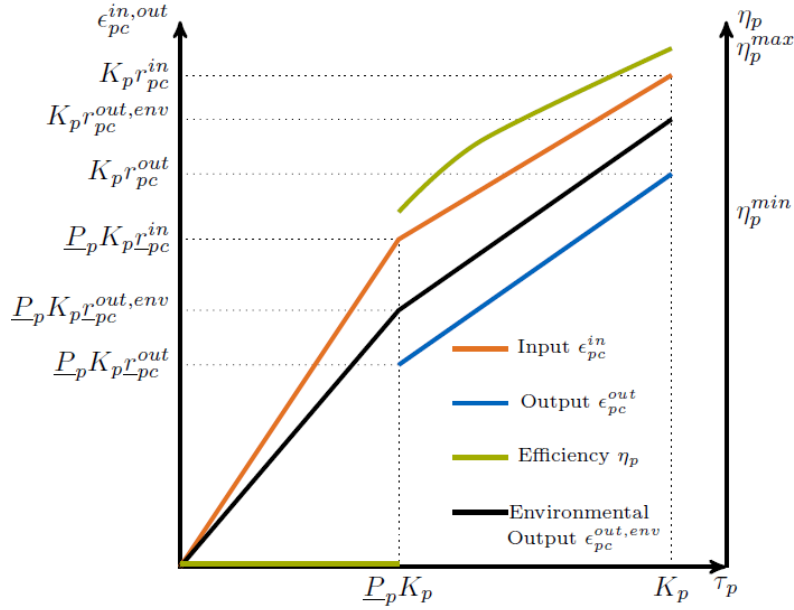

Coupling the throughput and the on/off marker: The following equation introduces a coupling between p_t , the boolean on/off marker of a process and its throughput τ_{pt} , so that p_t assumes the value 1 when the process has a non-zero output and 0 otherwise.

$$\forall p \in P^{\text{on/off}}, t \in T_m :$$

$$\underline{P}_p \cdot \kappa_p \cdot p_t \leq \tau_{pt} \leq \kappa_p \cdot p_t + \underline{P}_p \cdot \kappa_p \cdot (1 - p_t)$$

Input: The following equation describes the alteration of the input equation of a process with on/off and part-load behaviors due to the necessity of having a continuous, linear function defined on two intervals. The first interval represents the starting input of a process, while the second one represents the consumed

input while also producing.

$$\forall p \in P^{\text{on/off with part load}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{in}} = \tau_{pt} \cdot r_{pc}^{\text{in}} \cdot (1 - p_t) + \Delta t \cdot \left(\frac{r_{pc}^{\text{in}} - \underline{r}_{pc}^{\text{in}}}{1 - \underline{P}_p} \cdot \underline{P}_p \cdot \kappa_p + \frac{r_{pc}^{\text{in}} - \underline{P}_p \underline{r}_{pc}^{\text{in}}}{1 - \underline{P}_p} \cdot \tau_{pt} \right) \cdot p_t.$$

In order to ensure the continuity property of the function, the input ratio used for the starting interval has to be one corresponding to the minimum partial load, using $\underline{r}_{pc}^{\text{in}}$. This is a realistic value, since processes normally use, percentage-wise, more fuel in relationship to the throughput when starting than at higher throughput values.

Output differentiation: The following equations differentiate whether an output commodity needs to be produced when a process is starting (e.g. environmental commodities) or not (e.g. electricity):

$$\forall p \in P^{\text{on/off}}, c \in C^{\text{environmental}}, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} = \tau_{pt} \cdot r_{pc}^{\text{out}}$$

$$\forall p \in P^{\text{on/off}}, c \in C^{\text{non-environmental}}, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} = \tau_{pt} \cdot r_{pc}^{\text{out}} \cdot p_t.$$

If the process also shows part-load behavior, the previous two equations change to a similarly adapted version of the part-load output equation:

$$\forall p \in P^{\text{on/off with part load}}, c \in C^{\text{environmental}}, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} = \tau_{pt} \cdot r_{pc}^{\text{out}} \cdot (1 - p_t) + \Delta t \cdot \left(\frac{r_{pc}^{\text{out}} - r_{pc}^{\text{out}}}{1 - \underline{P}_p} \cdot \underline{P}_p \cdot \kappa_p + \frac{r_{pc}^{\text{out}} - \underline{P}_p r_{pc}^{\text{out}}}{1 - \underline{P}_p} \cdot \tau_{pt} \right) \cdot p_t$$

$$\forall p \in P^{\text{on/off}}, c \in C^{\text{non-environmental}}, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} = \Delta t \cdot \left(\frac{r_{pc}^{\text{out}} - r_{pc}^{\text{out}}}{1 - \underline{P}_p} \cdot \underline{P}_p \cdot \kappa_p + \frac{r_{pc}^{\text{out}} - \underline{P}_p r_{pc}^{\text{out}}}{1 - \underline{P}_p} \cdot \tau_{pt} \right) \cdot p_t.$$

Here, it is important to notice that the output of the environmental commodities becomes a continuous, piecewise linear function defined on two intervals. In order to ensure the continuity property of the function, the output ratio used for the starting interval has to be the partial one, $\underline{r}_{pc}^{\text{in}}$. This is a realistic value, since processes normally produce, percentage-wise, more CO2 and/or other environmental commodities in relationship to the throughput when starting then at higher throughput values.

Output ramping-up limit: While ramping up a process which can be turned on and off with a defined ramping up gradient, the following unrealistic situation might occur: Due to the fact that in the minimum working point the process on/off marker p_t can be both 0 and 1, the output of a process might have unrealistic jumps after the starting process is completed. There are 3 possible cases, each solved with its own output ramping equation, as follows:

Case I: When

$$\begin{aligned} \underline{P}_p &\geq \overline{PG}_p^{\text{up}} \\ \underline{P}_p &\text{ is a multiple of } \overline{PG}_p^{\text{up}}. \end{aligned}$$

Here, in order to ensure that the process behaves realistically, it is needed to ensure that the process starts producing in the minimum working point, $\underline{P}_p \kappa_p r_{pc}^{\text{out}}$, and not at a higher value. This is done by the following equation:

$$\forall p \in P^{\text{on/off, case I}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \underline{P}_p \kappa_p r_{pc}^{\text{out}}.$$

If the process shows a part load behavior, the equation changes to:

$$\forall p \in P^{\text{on/off with part load, case I}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \underline{P}_p \kappa_p r_{pc}^{\text{out}}.$$

If the process has a time variable efficiency, the equation changes to:

$$\forall p \in P^{\text{on/off with TimeVarEff, case I}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \underline{P}_p \kappa_p r_{pc}^{\text{out}} f_{pt}^{\text{out}}.$$

If the process has both a part load behavior and a time variable efficiency, the equation changes to:

$$\forall p \in P^{\text{on/off with TimeVarEff, case I}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \underline{P}_p \kappa_p r_{pc}^{\text{out}} f_{pt}^{\text{out}}.$$

Case II: When

$$\begin{aligned} \underline{P}_p &> \overline{PG}_p^{\text{up}} \\ \underline{P}_p &\text{ is not a multiple of } \overline{PG}_p^{\text{up}}. \end{aligned}$$

Here, in order to ensure that the process behaves realistically, it is needed to ensure that the process starts somewhere in the interval between the minimum working point $\underline{P}_p \kappa_p$ and the point of the first multiple of $\overline{PG}_p^{\text{up}}$ greater than $\underline{P}_p \kappa_p$, which is $(\frac{\underline{P}_p}{\overline{PG}_p^{\text{up}}} + 1) \cdot \overline{PG}_p$, where $\frac{\underline{P}_p}{\overline{PG}_p^{\text{up}}}$ is the rounded down number. This is done by the following equation:

$$\forall p \in P^{\text{on/off, case II}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \left(\frac{\underline{P}_p}{\overline{PG}_p^{\text{up}}} + 1 \right) \overline{PG}_p \kappa_p r_{pc}^{\text{out}}.$$

If the process shows a part load behavior, the equation changes to:

$$\forall p \in P^{\text{on/off, case II}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \left(\frac{\underline{P}_p}{\overline{PG}_p^{\text{up}}} + 1 \right) \overline{PG}_p \kappa_p r_{pc}^{\text{out}}.$$

If the process has a time variable efficiency, the equation changes to:

$$\forall p \in P^{\text{on/off with TimeVarEff, case II}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \left(\frac{\underline{P}_p}{\overline{PG}_p^{\text{up}}} + 1 \right) \overline{PG}_p \kappa_p r_{pc}^{\text{out}} f_{pt}^{\text{out}}.$$

If the process has both a part load behavior and a time variable efficiency, the equation changes to:

$$\forall p \in P^{\text{on/off with part load and TimeVarEff, case II}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \left(\frac{P_p}{\overline{PG}_p^{\text{up}}} + 1 \right) \overline{PG}_p \kappa_p r_{pc}^{\text{out}} f_{pt}^{\text{out}}.$$

Case III: When

$$\underline{P}_p < \overline{PG}_p^{\text{up}}.$$

Here, in order to ensure that the process behaves realistically, it is needed to ensure that the process starts somewhere in the interval between the minimum working point $\underline{P}_p \kappa_p$ and the first ramping up point greater than 0, $\overline{PG}_p^{\text{up}} \kappa_p$. This is done by the following equation:

$$\forall p \in P^{\text{on/off, case III}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \overline{PG}_p^{\text{up}} \kappa_p r_{pc}^{\text{out}}.$$

If the process shows a part load behavior, the equation changes to:

$$\forall p \in P^{\text{on/off, case III}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \overline{PG}_p^{\text{up}} \kappa_p r_{pc}^{\text{out}}.$$

If the process has a time variable efficiency, the equation changes to:

$$\forall p \in P^{\text{on/off with TimeVarEff, case III}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \overline{PG}_p^{\text{up}} \kappa_p r_{pc}^{\text{out}} f_{pt}^{\text{out}}.$$

If the process has both a part load behavior and a time variable efficiency, the equation changes to:

$$\forall p \in P^{\text{on/off with part load and TimeVarEff, case III}}, c \in C, t \in T_m :$$

$$\epsilon_{pct}^{\text{out}} - \epsilon_{pc(t-1)}^{\text{out}} \leq \Delta t \overline{PG}_p^{\text{up}} \kappa_p r_{pc}^{\text{out}} f_{pt}^{\text{out}}.$$

Starting ramp-up: There are some processes which have a different ramping up gradient while starting than while producing. This is usually defined with the help of a so called starting time. The following equations transform the starting time into a starting ramp and implement the starting ramp only during start, either as the only ramping constraint when no ramp up gradient is defined or by replacing during start the ramping up constraint which uses the ramping up gradient:

$$\forall p \in P^{\text{on/off with start time}}, t \in T_m :$$

$$SR_p = \frac{P_p}{ST_p}$$

$$\tau_{pt} - \tau_{p(t-1)} \leq \Delta t \overline{PG}_p^{\text{up}} \kappa_p p_{(t-1)} + \Delta t SR_p \kappa_p (1 - p_{(t-1)}).$$

Start-up costs: For those processes which have a fix start-up cost, it is necessary to identify whether a process has completed its starting phase and begins to produce or not. The following equation does

this by turning the boolean variable process start-up marker σ_{pt} to 1 when the process on/off marker switches from 0 to 1:

$$\forall p \in P^{\text{on/off with start cost}}, t \in T_m :$$

$$\sigma_{pt} \geq p_t - p_{(t-1)}.$$

The following table shows the possible values of σ_{pt} : .. table:: *Table: Process Start-up Marker Values*

pt	$p_{(t-1)}$	σ_{pt}
0	0	0 or 1 (0 is optimal)
0	1	0
1	0	1
1	1	0

Costs

The cost function is ammended with one cost type, the start-up cost:

$$\zeta = \zeta_{\text{inv}} + \zeta_{\text{fix}} + \zeta_{\text{var}} + \zeta_{\text{fuel}} + \zeta_{\text{startup}} + \zeta_{\text{env}}.$$

Turning on a process requires sometime an additional fix cost besides the fuel used for the starting. As the variable costs, these costs occur when processes are used:

$$\zeta_{\text{startup}} = w\Delta t \sum_{t \in T_m} p \in P_{\text{on/off}} P_p^{\text{start}} \sigma_{pt},$$

where P_p^{start} is the fix start-up cost and σ_{pt} is the process start-up marker. This cost type can also be merged into the same class of costs as the variable and fuel costs.

1.3 Technical documentation

Continue here if you want to understand in detail the model generator implementation.

1.3.1 Model Implementation

In this Section the **implementation** of the theoretical concepts of the model is described. This includes listing and describing all relevant sets, parameters, variables and constraints linking mathematical notation with the corresponding code fragment.

Sets

Since urbs is a linear optimization model with many objects (e.g variables, parameters), it is reasonable to use sets to define the groups of objects. With the usage of sets, many facilities are provided, such as understanding the main concepts of the model. Many objects are represented by various sets, therefore sets can be easily used to check whether some object has a specific characteristic or not. Additionally sets are useful to define a hierarchy of objects. Mathematical notation of sets are expressed with uppercase letters, and their members are usually expressed with the same lowercase letters. Main sets, tuple sets and subsets will be introduced in this respective order.

Elementary sets

Table 3: Table: Model Sets

Set	Description
$t \in T$	Timesteps
$t \in T_m$	Modelled Timesteps
$y \in Y$	Support timeframes
$v \in V$	Sites
$c \in C$	Commodities
$q \in Q$	Commodity Types
$p \in P$	Processes
$s \in S$	Storages
$f \in F$	Transmissions
$r \in R$	Cost Types

Time Steps

The model urbs is considered to observe a energy system model and calculate the optimal solution within a limited span of time. This limited span of time is viewed as a discrete variable, which means values of variables are viewed as occurring only at distinct timesteps. The set of **time steps** $T = \{t_0, \dots, t_N\}$ for N in \mathbb{N} represents Time. This set contains $N + 1$ sequential time steps with equal spaces. Each time step represents another point in time. At the initialisation of the model this set is fixed by the user by setting the variable `timesteps` in script `runme.py`. Duration of space between timesteps $\Delta t = t_{x+1} - t_x$, length of simulation $\Delta t \cdot N$ and time interval $[t_0, t_N]$ can be fixed to satisfy the needs of the user. In code this set is defined by the set `t` and initialized by the section:

```
m.t = pyomo.Set(  
    initialize=m.timesteps,  
    ordered=True,  
    doc='Set of timesteps')
```

Where:

- *Initialize*: A function that receives the set indices and model to return the value of that set element, initializes the set with data.
- *Ordered*: A boolean value that indicates whether the set is ordered.
- *Doc*: A string describing the set.

Modelled Timesteps

The Set, **modelled timesteps**, is a subset of the time steps set. The only difference between modelled timesteps set and the timesteps set is that the initial timestep t_0 is not included. All other features of the set time steps also apply to the set of modelled timesteps. This set is the main time set used in the model. The distinction with the set **timesteps** is only required to facilitate the definition of the storage state equation. In script `model.py` this set is defined by the set `tm` and initialized by the code fragment:

```
m.tm = pyomo.Set(
    within=m.t,
    initialize=m.timesteps[1:],
    ordered=True,
    doc='Set of modelled timesteps')
```

Where:

- *Within*: The option that supports the validation of a set array.
- `m.timesteps[1:]` represents the timesteps set starting from the second element, excluding the first timestep t_0

Support timeframes

Support timeframes are represented by the set Y . They represent the explicitly modeled support timeframes, e.g., years, for intertemporal models. In script `model.py` the set is defined as:

```
m.stf = pyomo.Set(
    initialize=(m.commodity.index.get_level_values('support_timeframe')
                .unique()),
    doc='Set of modeled support timeframes (e.g. years)')
```

Sites

Sites are represented by the set V . A Site v can be any distinct location, a place of settlement or activity (e.g *process*, *transmission*, *storage*). A site is for example an individual building, region, country or even continent. Sites can be imagined as nodes(vertices) on a graph of locations, connected by edges. Index of this set are the descriptions of the Sites (e.g north, middle, south). In script `model.py` this set is defined by `sit` and initialized by the code fragment:

```
m.sit = pyomo.Set(
    initialize=m.commodity.index.get_level_values('Site').unique(),
    doc='Set of sites')
```

Commodities

As explained in the Overview section, **commodities** are goods that can be generated, stored, transmitted or consumed. The set of Commodities represents all goods that are relevant to the modelled energy system, such as all energy carriers, inputs, outputs, intermediate substances. (e.g Coal, CO2, Electric, Wind) By default, commodities are given by their energy content (MWh). Usage of some commodities are limited by a maximum value or maximum value per timestep due to their availability or restrictions, also some commodities have a price that needs to be compensated..(e.g coal, wind, solar).In script `model.py` this set is defined by `com` and initialized by the code fragment:

```
m.com = pyomo.Set(
    initialize=m.commodity.index.get_level_values('Commodity').unique(),
    doc='Set of commodities')
```

Commodity Types

Commodities differ in their usage purposes, consequently **commodity types** are introduced to subdivide commodities by their features. These Types are hard coded as SupIm, Stock, Demand, Env, Buy, Sell. In script `model.py` this set is defined as `com_type` and initialized by the code fragment:

```
m.com_type = pyomo.Set(  
    initialize=m.commodity.index.get_level_values('Type').unique(),  
    doc='Set of commodity types')
```

Processes

One of the most important elements of an energy system is the **process**. A process p can be defined by the action of changing one or more forms of energy, i.e. commodities, to others. In our modelled energy system, processes convert input commodities into output commodities. Process technologies are represented by the set processes P . Different processes technologies have fixed input and output commodities. These input and output commodities can be either single or multiple regardless of each other. Some example members of this set can be: *Wind Turbine*, *Gas Plant*, *Photovoltaics*. In script `model.py` this set is defined as `pro` and initialized by the code fragment:

```
m.pro = pyomo.Set(  
    initialize=m.process.index.get_level_values('Process').unique(),  
    doc='Set of conversion processes')
```

Storages

Energy **Storage** is provided by technical facilities that store energy to generate a commodity at a later time for the purpose of meeting the demand. Occasionally, on-hand commodities may not be able to satisfy the required amount of energy to meet the demand, or the available amount of energy may be much more than required. Storage technologies play a major role in such circumstances. The Set S represents all storage technologies (e.g *Pump storage*). In script `model.py` this set is defined as `sto` and initialized by the code fragment:

```
m.sto = pyomo.Set(  
    initialize=m.storage.index.get_level_values('Storage').unique(),  
    doc='Set of storage technologies')
```

Transmissions

Transmissions $f \in F$ represent possible conveyances of commodities between sites. Transmission process technologies can vary between different commodities, due to distinct physical attributes and forms of commodities. Some examples for Transmission technologies are: *hvac*, *hvdc*, *pipeline*) In script `model.py` this set is defined as `tra` and initialized by the code fragment:

```
m.tra = pyomo.Set(  
    initialize=m.transmission.index.get_level_values('Transmission').  
    ↪unique(),  
    doc='Set of transmission technologies')
```


Cost Types

One of the major goals of the model is to calculate the costs of a simulated energy system. There are 6 different types of costs. Each one has different features and are defined for different instances. Set of **cost types** is hardcoded, which means they are not considered to be fixed or changed by the user. The Set R defines the Cost Types, each member r of this set R represents a unique cost type name. The cost types are hard coded as: Investment, Fix, Variable, Fuel, Revenue, Purchase, Startup. In script `model.py` this set is defined as `cost_type` and initialized by the code fragment:

```
m.cost_type = pyomo.Set(
    initialize=['Inv', 'Fix', 'Var', 'Fuel', 'Revenue', 'Purchase', 'Startup'
    → ],
    doc='Set of cost types (hard-coded)')
```

Tuple Sets

A tuple is finite, ordered collection of elements. For example, the tuple `(hat, red, large)` consists of 3 ordered elements and defines another element itself. Tuples are needed in this model to define the combinations of elements from different sets. Defining a tuple lets us assemble related elements and use them as a single element. These tuples are then collected into tuple sets. These tuple sets are then immensely useful for efficient indexing of model variables and parameters and for defining the constraint rules.

Commodity Tuples

Commodity tuples represent combinations of defined commodities. These are represented by the set $C_{y v q}$. A member $c_{y v q}$ in set $C_{y v q}$ is a commodity c of commodity type q in support timeframe y and site v . For example, `(2020, Mid, Elec, Demand)` is interpreted as commodity *Elec* of commodity type *Demand* in the year 2020 in site *Mid*. This set is defined as `com_tuples` and given by the code fragment:

```
m.com_tuples = pyomo.Set(
    within=m.stf*m.sit*m.com*m.com_type,
    initialize=m.commodity.index,
    doc='Combinations of defined commodities, e.g. (2020,Mid,Elec,Demand)')
```

Process Tuples

Process tuples represent possible placements of processes within the model. These are represented by the set P_v . A member $p_{y v}$ in set $P_{y v}$ is a process p in support timeframe y and site v . For example, `(2020, North, Coal Plant)` is interpreted as process *Coal Plant* in site *North* in the year 2020. This set is defined as `pro_tuples` and given by the code fragment:

```
m.pro_tuples = pyomo.Set(
    within=m.stf*m.sit*m.pro,
    initialize=m.process.index,
    doc='Combinations of possible processes, e.g. (2020,North,Coal plant)')
```

There are several subsets defined for process tuples, which each activate a different set of modeling constraints.

The first subset is formed in order to capture all processes that take up a certain area and are thus subject to the area constraint at the given site. These processes are identified by the parameter `area-per-cap` set in table *Process*, if at the same time a value for `area` is set in table *Site*. The tuple set is defined as:

```
m.pro_area_tuples = pyomo.Set(
    within=m.stf*m.sit*m.pro,
    initialize=m.proc_area.index,
    doc='Processes and Sites with area Restriction')
```

The second subset is formed in order to capture all processes which have the parameter `process new capacity block` K_{yvp}^{block} set in the table *Process*, used for building new capacity in blocks. The tuple set is defined as:

```
m.pro_cap_new_block_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, site, process)
        for (stf, site, process) in m.pro_tuples
        for (s, si, pro) in tuple(m.cap_block_dict.keys())
        if process == pro and si == site and s == stf],
    doc='Processes with new capacities built in blocks')
```

The third subset of the process tuples `pro_minfraction_tuples` $P_{yv}^{\text{minfraction}}$ is formed in order to identify processes that have a minimum fraction defined without having partial operation properties and cannot be turned off. Programatically, they are identified by those processes which have the parameter `min-fraction` set and the parameter `on-off` set to 0 in the table *Process*. The tuple set is defined in *AdvancedProcesses.py* as:

```
m.pro_minfraction_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, site, process)
        for (stf, site, process) in m.pro_tuples
        for (st, sit, pro) in tuple(m.min_fraction_dict.keys())
        if stf == st and sit == site and process == pro and
        m.process_dict['on-off'][stf, site, process] != 1],
    doc='Processes with constant efficiency and minimum working load which'
        'cannot be turned off')
```

The fourth subset of the process tuples `pro_partial_tuples` P_{yv}^{partial} is formed in order to identify processes that have partial operation properties and cannot be turned off. Programmatically, they are identified by those processes, which have the parameter `ratio-min` set for one of their input and/or output commodities in table *Process-Commodity* and the parameter `on-off` in the table *Process* set to 0. The tuple set is defined in *AdvancedProcesses.py* as:

```
m.pro_partial_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, site, process)
        for (stf, site, process) in m.pro_tuples
        for (s, pro, _) in tuple(m.r_in_min_fraction_dict.keys() or
                                m.r_out_min_fraction_dict.keys())
        if process == pro and s == stf and
        m.process_dict['on-off'][stf, site, process] != 1],
    doc='Processes with partial input/output which cannot be turned off')
```

The fifth subset of the process tuples `pro_on_off_tuples` $P_{yv}^{on/off}$ is formed in order to identify processes that have a minimum fraction defined without having partial operation properties and can be turned off. Programmatically, they are identified by those processes which have the parameter `min-fraction` set and the parameter `on-off` set to 1 in the table *Process*. The tuple set is defined in `AdvancedProcesses.py` as:

```
m.pro_on_off_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, site, process)
                 for (stf, site, process) in
                     tuple(m.min_fraction_dict.keys())
                 for (st, sit, pro) in tuple(m.onoff_dict.keys())
                 if stf == st and site == sit and process == pro],
    doc='Processes with minimal fraction which can be turned off')
```

The sixth subset of the process tuples `pro_on_off_partial_tuples` $P_{yv}^{partial\ on/off}$ is formed in order to identify processes that have a minimum fraction defined, partial operation properties and can be turned off. Programmatically, they are identified by those processes, which have the parameter `ratio-min` set for one of their input and/or output commodities in table *Process-Commodity* and the parameter `on-off` in the table *Process* set to 1. The tuple set is defined in `AdvancedProcesses.py` as:

```
m.pro_partial_on_off_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, site, process)
                 for (stf, site, process) in m.pro_tuples
                 for (st, pro, _) in tuple(m.r_in_min_fraction_dict.keys())
                                     or m.r_out_min_fraction_dict)
                 if process == pro and stf == st and
                 m.process_dict['on-off'][stf, site, process] == 1],
    doc='Processes with partial input/output which can be turned off')
```

Finally, processes that are subject to restrictions in the change of operational state are captured with the `pro_rampupgrad_tuples` and `pro_rampdowngrad_tuples`. This subsets are defined in `AdvancedProcesses` as:

```
m.pro_rampupgrad_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, sit, pro)
                 for (stf, sit, pro) in m.pro_tuples
                 if m.process_dict['ramp-up-grad'][stf, sit, pro] < 1.0 /
↪dt],
    doc='Processes with maximum ramp up gradient smaller than timestep_
↪length')
```

```
m.pro_rampdowngrad_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, sit, pro)
                 for (stf, sit, pro) in m.pro_tuples
                 if m.process_dict['ramp-down-grad'][stf, sit, pro] < 1.0 /
↪dt],
    doc='Processes with maximum ramp down gradient smaller than timestep_
↪length')
```

In the case of a process which can be turned on and off and are subject to restrictions in the change of operational state while starting are captured with the `pro_rampup_start_tuples`, subset which is defined in `advancedProcesses.py` as:

```
m.pro_rampup_start_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro,
    initialize=[(stf, sit, pro)
                 for (stf, sit, pro) in m.pro_on_off_tuples
                 if m.process_dict['start-time'][stf, sit, pro]
                    > 1.0 / m.dt],
    doc='Processes with different starting ramp up gradient')
```

Transmission Tuples

Transmission tuples represent possible transmissions. These are represented by the set $F_{ycv_{out}v_{in}}$. A member $f_{ycv_{out}v_{in}}$ in set $F_{ycv_{out}v_{in}}$ is a transmission f , that is directed from an origin site v_{out} to a destination site v_{in} and carrying the commodity c in support timeframe y . The term “directed from an origin site v_{out} to a destination site v_{in} ” can also be defined as an arc a . For example, (2020, South, Mid, hvac, Elec) is interpreted as transmission hvac that is directed from origin site South to destination site Mid carrying commodity Elec in year 2020. This set is defined as tra_tuples and given by the code fragment:

```
m.tra_tuples = pyomo.Set(
    within=m.stf*m.sit*m.sit*m.tra*m.com,
    initialize=m.transmission.index,
    doc='Combinations of possible transmissions, e.g. '
        '(2020, South, Mid, hvac, Elec) ')
```

The set $F_{ycv_{out}v_{in}}^{blocks}$ includes all transmission lines which have a defined capacity block for the building of new transmission capacities.

```
m.tra_block_tuples = pyomo.Set(
    within=m.stf * m.sit * m.sit * m.tra * m.com,
    initialize=[(stf, sit, sit_, tra, com)
                 for (stf, sit, sit_, tra, com) in tuple(m.tra_block_dict.
    ↪keys())],
    doc='Transmission with new block capacities')
```

DCPF Transmission Tuples

If the DC Power Flow Model feature is activated in the model, three different transmission tuple sets are defined in the model.

The set $F_{ycv_{out}v_{in}}^{TP}$ includes every transport model transmission lines and is defined as tra_tuples_tp and given by the code fragment:

```
m.tra_tuples_tp = pyomo.Set(
    within=m.stf * m.sit * m.sit * m.tra * m.com,
    initialize=tuple(tra_tuples_tp),
    doc='Combinations of possible transport transmissions, '
        'e.g. (2020, South, Mid, hvac, Elec) ')
```

The set $F_{ycv_{out}v_{in}}^{DCPF}$ includes every transmission line, which should be modelled with DCPF. If the complementary arcs are included in the input for DCPF transmission lines, these will be excluded from this set with remove_duplicate_transmission(). This set is defined as tra_tuples_dc and given by the code fragment:

```
m.tra_tuples_dc = pyomo.Set(
    within=m.stf * m.sit * m.sit * m.tra * m.com,
    initialize=tuple(tra_tuples_dc),
    doc='Combinations of possible bidirectional dc'
        'transmissions, e.g. (2020, South, Mid, hvac, Elec)')

```

If the DCPF is activated, the set $F_{y^{cv_{out}v_{in}}}$ is defined by the unification of the sets $F_{y^{cv_{out}v_{in}}^{DCPF}}$ and $F_{y^{cv_{out}v_{in}}^{TP}}$. This set is defined as `tra_tuples` in the same fashion as the default transmission model.

Storage Tuples

Storage tuples label storages. They are represented by the set S_{yvc} . A member s_{yvc} in set S_{yvc} is a storage s of commodity c in site v and support timeframe y . For example, $(2020, Mid, Bat, Elec)$ is interpreted as storage *Bat* for commodity *Elec* in site *Mid* in the year 2020. This set is defined as `sto_tuples` and given by the code fragment:

```
m.sto_tuples = pyomo.Set(
    within=m.stf*m.sit*m.sto*m.com,
    initialize=m.storage.index,
    doc='Combinations of possible storage by site,'
        'e.g. (2020, Mid, Bat, Elec)')

```

There are four subsets of storage tuples.

In a first subset of the storage tuples are all storages that have a user defined fixed value for the initial state are collected.

```
m.sto_init_bound_tuples = pyomo.Set(
    within=m.stf*m.sit*m.sto*m.com,
    initialize=m.stor_init_bound.index,
    doc='storages with fixed initial state')

```

A second subset is defined for all storages that have a fixed ratio between charging/discharging power and storage content.

```
m.sto_ep_ratio_tuples = pyomo.Set(
    within=m.stf*m.sit*m.sto*m.com,
    initialize=tuple(m.sto_ep_ratio_dict.keys()),
    doc='storages with given energy to power ratio')

```

The third and fourth subsets are defined for all the storages that have a capacity or power expansion block defined in the input.

```
m.sto_block_c_tuples = pyomo.Set(
    within=m.stf * m.sit * m.sto * m.com,
    initialize=tuple(m.sto_block_c_dict.keys()),
    doc='storages with new energy block capacities')
m.sto_block_p_tuples = pyomo.Set(
    within=m.stf * m.sit * m.sto * m.com,
    initialize=tuple(m.sto_block_p_dict.keys()),
    doc='storages with new power block capacities')

```

Process Input Tuples

Process input tuples represent commodities consumed by processes. These are represented by the set C_{yvp}^{in} . A member c_{yvp}^{in} in set C_{yvp}^{in} is a commodity c consumed by the process p in site v in support timeframe y . For example, $(2020, \text{Mid}, \text{PV}, \text{Solar})$ is interpreted as commodity *Solar* consumed by the process *PV* in the site *Mid* in the year 2020. This set is defined as `pro_input_tuples` and given by the code fragment:

```
m.pro_input_tuples = pyomo.Set(
    within=m.stf*m.sit*m.pro*m.com,
    initialize=[(stf, site, process, commodity)
                 for (stf, site, process) in m.pro_tuples
                 for (s, pro, commodity) in m.r_in.index
                 if process == pro and s == stf],
    doc='Commodities consumed by process by site, '
        'e.g. (2020,Mid,PV,Solar)')
```

Where: `r_in` represents the process input ratio as set in the input.

For processes in the tuple set `pro_partial_tuples`, the following tuple set `pro_partial_input_tuples` enumerates their input commodities. It is used to index the constraints that modifies a process' input commodity flow with respect to the standard case without partial operation. It is defined by the following code fragment:

```
m.pro_partial_input_tuples = pyomo.Set(
    within=m.stf*m.sit*m.pro*m.com,
    initialize=[(stf, site, process, commodity)
                 for (stf, site, process) in m.pro_partial_tuples
                 for (s, pro, commodity) in m.r_in_min_fraction.index
                 if process == pro and s == stf],
    doc='Commodities with partial input ratio, '
        'e.g. (2020,Mid,Coal PP,Coal)')
```

Where: `r_in_min_fraction` represents the process input ratio as set in the input for the minimum load of the process.

For processes in the tuple set `pro_on_off_tuples`, the following tuple set `pro_on_off_input_tuples` enumerates their input commodities. It is used to index the constraints that modifies a process' input commodity flow with respect to the standard case without the on/off feature. It is defined by the following code fragment in `AdvancedProcesses.py`:

```
m.pro_on_off_input_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro * m.com,
    initialize=[(stf, site, process, commodity)
                 for (stf, site, process) in m.pro_on_off_tuples
                 for (s, pro, commodity) in tuple(m.r_in_dict.keys())
                 if process == pro and stf == s],
    doc='Commodities for on/off input')
```

For processes in the tuple set `pro_partial_on_off_tuples`, the following tuple set `pro_partial_on_off_input_tuples` enumerates their input commodities. It is used to index the constraints that modifies a process' input commodity flow with respect to the standard case without the on/off feature and partial operation. It is defined by the following code fragment in `AdvancedProcesses.py`:

```
m.pro_partial_on_off_input_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro * m.com,
    initialize=[(stf, site, process, commodity)
                 for (stf, site, process) in m.pro_partial_on_off_tuples
                 for (s, pro, commodity) in tuple(m.r_in_min_fraction_dict
                                                  .keys())

                 if process == pro and s == stf],
    doc='Commodities with partial input ratio which can be turned off,'
        'e.g. (2020,Mid,Coal PP,Coal)')

```

Process Output Tuples

Process output tuples represent commodities generated by processes. These are represented by the set C_{yvp}^{out} . A member c_{yvp}^{out} in set C_{yvp}^{out} is a commodity c generated by the process p in site v and support timeframe y . For example, $(2020, \text{Mid}, \text{PV}, \text{Elec})$ is interpreted as the commodity *Elec* is generated by the process *PV* in the site *Mid* in the year 2020. This set is defined as `pro_output_tuples` and given by the code fragment:

```
m.pro_output_tuples = pyomo.Set(
    within=m.stf*m.sit*m.pro*m.com,
    initialize=[(stf, site, process, commodity)
                 for (stf, site, process) in m.pro_tuples
                 for (s, pro, commodity) in m.r_out.index
                 if process == pro and s == stf],
    doc='Commodities produced by process by site, e.g. (2020,Mid,PV,Elec)')

```

Where: `r_out` represents the process output ratio as set in the input.

There are several alternative tuple sets that are active whenever their respective features are set in the input.

First, for processes in the tuple set `pro_partial_tuples`, the tuple set `pro_partial_output_tuples` enumerates their output commodities. It is used to index the constraints that modifies a process' output commodity flow with respect to the standard case without partial operation. It is defined by the following code fragment:

```
m.pro_partial_output_tuples = pyomo.Set(
    within=m.stf*m.sit*m.pro*m.com,
    initialize=[(stf, site, process, commodity)
                 for (stf, site, process) in m.pro_partial_tuples
                 for (s, pro, commodity) in m.r_out_min_fraction.index
                 if process == pro and s == stf],
    doc='Commodities with partial input ratio, e.g. (Mid,Coal PP,CO2)')

```

Second, for processes in the tuple set `pro_on_off_tuples`, the tuple set `pro_on_off_output_tuples` enumerates their output commodities. It is used to index the constraints that modifies a process' output commodity flow with respect to the standard case without the on/off feature. It is defined by the following code fragment in `AdvancedProcesses.py`:

```
m.pro_on_off_output_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro * m.com,
    initialize=[(stf, site, process, commodity)
                 for (stf, site, process) in m.pro_on_off_tuples

```

(continues on next page)

(continued from previous page)

```

        for (s, pro, commodity) in tuple(m.r_out_dict.keys())
        if process == pro and stf == s],
    doc='Commodities for on/off output')

```

Third, for processes in the tuple set `pro_partial_on_off_tuples`, the tuple set `pro_partial_on_off_output_tuples` enumerates their output commodities. It is used to index the constraints that modifies a process' output commodity flow with respect to the standard case without the on/off feature and partial operation. It is defined by the following code fragment in `AdvancedProcesses.py`:

```

m.pro_partial_on_off_output_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro * m.com,
    initialize=[(stf, site, process, commodity)
        for (stf, site, process) in m.pro_partial_on_off_tuples
        for (s, pro, commodity) in tuple(m.r_out_min_fraction_
→dict
                                                .keys())
        if process == pro and s == stf],
    doc='Commodities for on/off output with partial behaviour')

```

Fourth, the processes in the tuple sets `pro_on_off_tuples` and `pro_partial_on_off_tuples` require another constraint to limit the excessive growth of the output of a process. This is required due to the fact that in the point of minimum load, without these limiting constraints, the process on/off marker *yvpt* can be both on and off. There are three cases to be considered:

The first case is represented by the tuple set `pro_rampup_divides_minfraction_output_tuples`, which covers the outputs of the processes for which the defined ramp up gradient and is smaller than the minimum load fraction and is a divisor of it. It is defined by the following code fragment in `AdvancedProcesses.py`:

```

m.pro_rampup_divides_minfraction_output_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro * m.com,
    initialize=[(stf, sit, pro, com)
        for (stf, sit, pro, com) in m.pro_on_off_output_tuples
        if m.process_dict['ramp-up-grad'][stf, sit, pro] < 1.0 / m.
→dt and
        m.process_dict['ramp-up-grad'][stf, sit, pro] <=
        m.min_fraction_dict[stf, sit, pro] and
        m.min_fraction_dict[stf, sit, pro] %
        m.process_dict['ramp-up-grad'][stf, sit, pro] == 0 and
        com not in m.com_env],
    doc='Output commodities of processes with ramp-up-grad smaller than '
        'timestep length and smaller equal than min-fraction and is a '
        'divisor of min-fraction')

```

The second case is represented by the tuple set `pro_rampup_not_divides_minfraction_output_tuples`, which covers the outputs of the processes for which the defined ramp up gradient and is smaller than the minimum load fraction and is not a divisor of it. It is defined by the following code fragment in `AdvancedProcesses.py`:

```

m.pro_rampup_not_divides_minfraction_output_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro * m.com,
    initialize=[(stf, sit, pro, com)

```

(continues on next page)

(continued from previous page)

```

        for (stf, sit, pro, com) in m.pro_on_off_output_tuples
        if m.process_dict['ramp-up-grad'][stf, sit, pro] < 1.0 / m.
→dt and
            m.process_dict['ramp-up-grad'][stf, sit, pro] <
            m.min_fraction_dict[stf, sit, pro] and
            m.min_fraction_dict[stf, sit, pro] %
            m.process_dict['ramp-up-grad'][stf, sit, pro] != 0 and
            com not in m.com_env],
    doc='Output commodities of processes with ramp-up-grad smaller than'
        'timestep length and smaller than min-fraction and is NOT a '
        'divisor of min-fraction')

```

The third and last case is represented by the tuple set `pro_rampup_bigger_minfraction_output_tuples`, which covers the outputs of the processes for which the defined ramp up gradient and is greater than the minimum load fraction. It is defined by the following code fragment in `AdvancedProcesses.py`:

```

m.pro_rampup_bigger_minfraction_output_tuples = pyomo.Set(
    within=m.stf * m.sit * m.pro * m.com,
    initialize=[(stf, sit, pro, com)
        for (stf, sit, pro, com) in m.pro_on_off_output_tuples
        if m.process_dict['ramp-up-grad'][stf, sit, pro] < 1.0 / m.
→dt and
            m.process_dict['ramp-up-grad'][stf, sit, pro] >
            m.min_fraction_dict[stf, sit, pro] and
            com not in m.com_env],
    doc='Output commodities of processes with ramp up gradient smaller'
        'than timestep length and greater than min-fraction')

```

Last, the output of all processes that have a time dependent efficiency are collected in an additional tuple set. The set contains all outputs corresponding to processes that are specified as column indices in the input file worksheet `TimeVarEff`.

```

m.pro_timevar_output_tuples = pyomo.Set(
    within=m.sit*m.pro*m.com,
    initialize=[(site, process, commodity)
        for (site, process) in m.eff_factor.columns.values
        for (pro, commodity) in m.r_out.index
        if process == pro],
    doc='Outputs of processes with time dependent efficiency')

```

Demand Side Management Tuples

There are two kinds of demand side management (DSM) tuples in the model: DSM site tuples D_{yvc} and DSM down tuples $D_{yvct,tt}^{\text{down}}$. The first kind D_{yvc} represents all possible combinations of support timeframe y , site v and commodity c of the DSM sheet. It is given by the code fragment:

```

m.dsm_site_tuples = pyomo.Set(
    within=m.stf*m.sit*m.com,
    initialize=m.dsm.index,
    doc='Combinations of possible dsm by site, e.g. (2020, Mid, Elec)')

```

The second kind $D_{t,tt,yvc}^{\text{down}}$ refers to all possible DSM downshift possibilities. It is defined to overcome the difficulty caused by the two time indices of the DSM downshift variable. Dependend on support

timeframe y , site v and commodity c the tuples contain two time indices. For example $(5001, 5003, 2020, Mid, Elec)$ is interpreted as the downshift in timestep 5003, which was caused by the upshift of timestep 5001 in year 2020 and 'site' *Mid* for commodity *Elec*. The tuples are given by the following code fragment:

```
m.dsm_down_tuples = pyomo.Set(
    within=m.tm*m.tm*m.stf*m.sit*m.com,
    initialize=[(t, tt, stf, site, commodity)
                 for (t, tt, stf, site, commodity)
                 in dsm_down_time_tuples(m.timesteps[1:],
                                         m.dsm_site_tuples,
                                         m)],
    doc='Combinations of possible dsm_down combinations, e.g. '
        '(5001,5003,2020,Mid,Elec)')
```

where the following function is utilized:

```
def dsm_down_time_tuples(time, sit_com_tuple, m):
    """ Dictionary for the two time instances of DSM_down
    Args:
        time: list with time indices
        sit_com_tuple: a list of (site, commodity) tuples
        m: model instance
    Returns:
        A list of possible time tuples depending on site and commodity
    """

    delay = m.dsm_dict['delay']
    ub = max(time)
    lb = min(time)
    time_list = []

    for (stf, site, commodity) in sit_com_tuple:
        for step1 in time:
            for step2 in range(step1 -
                               max(int(delay[stf, site, commodity] /
                                         m.dt.value), 1),
                               step1 +
                               max(int(delay[stf, site, commodity] /
                                         m.dt.value), 1) + 1):
                if lb <= step2 <= ub:
                    time_list.append((step1, step2, stf, site, commodity))

    return time_list
```

Commodity Type Subsets

Commodity Type Subsets represent the commodity tuples only from a given commodity type. Commodity Type Subsets are subsets of the sets commodity tuples. These subsets can be obtained by fixing the commodity type q to a desired commodity type (e.g. SupIm, Stock) in the set commodity tuples C_{vq} . Since there are 6 types of commodity types, there are also 6 commodity type subsets. Commodity type subsets are;

Supply Intermittent Commodities (SupIm): The set C_{sup} represents all commodities c of commodity type SupIm. Commodities of this type have intermittent timeseries, in other words, availability of these

commodities are not constant. These commodities might have various energy content for every timestep t . For example solar radiation is contingent on many factors such as sun position, weather and varies permanently.

Stock Commodities (Stock): The set C_{st} represents all commodities c of commodity type Stock. Commodities of this type can be purchased at any time for a given price(k_{vc}^{fuel}).

Sell Commodities (Sell): The set C_{sell} represents all commodities c of commodity type Sell. Commodities that can be sold. These Commodities have a sell price (k_{vct}^{bs}) that may vary with the given timestep t .

Buy Commodities (Buy): The set C_{buy} represents all commodities c of commodity type Buy. Commodities that can be purchased. These Commodities have a buy price (k_{vc}^{bs}) that may vary with the given timestep t .

Demand Commodities (Demand): The set C_{dem} represents all commodities c of commodity type Demand. Commodities of this type are the requested commodities of the energy system. They are usually the end product of the model (e.g Electricity:Elec).

Environmental Commodities (Env): The set C_{env} represents all commodities c of commodity type Env. Commodities of this type are usually the undesired byproducts of processes that might be harmful for environment, optional maximum creation limits can be set to control the generation of these commodities (e.g Greenhouse Gas Emissions: CO₂).

Commodity Type Subsets are given by the code fragment:

```
m.com_supim = pyomo.Set(
    within=m.com,
    initialize=commodity_subset(m.com_tuples, 'SupIm'),
    doc='Commodities that have intermittent (timeseries) input')
m.com_stock = pyomo.Set(
    within=m.com,
    initialize=commodity_subset(m.com_tuples, 'Stock'),
    doc='Commodities that can be purchased at some site(s)')
m.com_sell = pyomo.Set(
    within=m.com,
    initialize=commodity_subset(m.com_tuples, 'Sell'),
    doc='Commodities that can be sold')
m.com_buy = pyomo.Set(
    within=m.com,
    initialize=commodity_subset(m.com_tuples, 'Buy'),
    doc='Commodities that can be purchased')
m.com_demand = pyomo.Set(
    within=m.com,
    initialize=commodity_subset(m.com_tuples, 'Demand'),
    doc='Commodities that have a demand (implies timeseries)')
m.com_env = pyomo.Set(
    within=m.com,
    initialize=commodity_subset(m.com_tuples, 'Env'),
    doc='Commodities that (might) have a maximum creation limit')
```

Where:

`urbs.commodity_subset (com_tuples, type_name)`

Returns the commodity names(c) of the given commodity type(q).

Parameters

- **com_tuples** – A list of tuples (site, commodity, commodity type)

- **type_name** – A commodity type or a list of commodity types

Returns The set (unique elements/list) of commodity names of the desired commodity type.

Operational state tuples

For intertemporal optimization the operational state of units in a support timeframe y has to be calculated from both the initially installed units and their remaining lifetime and the units installed in a previous support timeframe which are still operational in y . This is achieved via 6 tuple sets two each for processes, transmissions and storages.

Initially installed units

Processes which are already installed at the beginning of the modeled time horizon and still operational in support timeframe stf are collected in the following tuple set:

```
m.inst_pro_tuples = pyomo.Set(
    within=m.sit*m.pro*m.stf,
    initialize=[(sit, pro, stf)
                 for (sit, pro, stf)
                 in inst_pro_tuples(m)],
    doc=' Installed processes that are still operational through stf')
```

where the following function is utilized:

```
def inst_pro_tuples(m):
    """ Tuples for operational status of already installed units
        (processes, transmissions, storages) for intertemporal planning.
        Only such tuples where the unit is still operational until the next
        support time frame are valid.
    """
    inst_pro = []
    sorted_stf = sorted(list(m.stf))

    for (stf, sit, pro) in m.inst_pro.index:
        for stf_later in sorted_stf:
            index_helper = sorted_stf.index(stf_later)
            if stf_later == max(m.stf):
                if (stf_later +
                    m.global_prop.loc[(max(sorted_stf), 'Weight'), 'value'])_
→-
                    1 < min(m.stf) + m.process_dict['lifetime'][(stf, sit, pro)]):
                    inst_pro.append((sit, pro, stf_later))
            elif (stf_later + sorted_stf[index_helper + 1]) / 2 <= (min(m.
→stf)
                                                                    + m.
→process_dict['lifetime'][(stf, sit, pro)]):
                    inst_pro.append((sit, pro, stf_later))

    return inst_pro
```

Transmissions which are already installed at the beginning of the modeled time horizon and still operational in support timeframe *stf* are collected in the following tuple set:

```
m.inst_tra_tuples = pyomo.Set(
    within=m.sit*m.sit*m.tra*m.com*m.stf,
    initialize=[(sit, sit_, tra, com, stf)
                 for (sit, sit_, tra, com, stf)
                 in inst_tra_tuples(m)],
    doc='Installed transmissions that are still operational through stf')
```

where the following function is utilized:

```
def inst_tra_tuples(m):
    """ s.a. inst_pro_tuples
    """
    inst_tra = []
    sorted_stf = sorted(list(m.stf))

    for (stf, sit1, sit2, tra, com) in m.inst_tra.index:
        for stf_later in sorted_stf:
            index_helper = sorted_stf.index(stf_later)
            if stf_later == max(m.stf):
                if (stf_later +
                    m.global_prop_dict['value'][(max(sorted_stf), 'Weight
→')] -
                    1 < min(m.stf) + m.transmission_dict['lifetime'][(
                        stf, sit1, sit2, tra, com)]):
                    inst_tra.append((sit1, sit2, tra, com, stf_later))
            elif (sorted_stf[index_helper + 1] <= min(m.stf) +
                  m.transmission_dict['lifetime'][(
                      stf, sit1, sit2, tra, com)]):
                    inst_tra.append((sit1, sit2, tra, com, stf_later))

    return inst_tra
```

Storages which are already installed at the beginning of the modeled time horizon and still operational in support timeframe *stf* are collected in the following tuple set:

```
m.inst_sto_tuples = pyomo.Set(
    within=m.sit*m.sto*m.com*m.stf,
    initialize=[(sit, sto, com, stf)
                 for (sit, sto, com, stf)
                 in inst_sto_tuples(m)],
    doc='Installed storages that are still operational through stf')
```

where the following function is utilized:

```
def inst_sto_tuples(m):
    """ s.a. inst_pro_tuples
    """
    inst_sto = []
    sorted_stf = sorted(list(m.stf))

    for (stf, sit, sto, com) in m.inst_sto.index:
        for stf_later in sorted_stf:
            index_helper = sorted_stf.index(stf_later)
            if stf_later == max(m.stf):
```

(continues on next page)

(continued from previous page)

```

        if (stf_later +
            m.global_prop_dict['value'][(max(sorted_stf), 'Weight
→')] -
            1 < min(m.stf) +
            m.storage_dict['lifetime'][(stf, sit, sto, com)]):
            inst_sto.append((sit, sto, com, stf_later))
        elif (sorted_stf[index_helper + 1] <=
            min(m.stf) + m.storage_dict['lifetime'][(stf, sit, sto, com)]):
            inst_sto.append((sit, sto, com, stf_later))

    return inst_sto

```

Installation in earlier support timeframe

Processes installed in an earlier support timeframe *stf* and still usable in support timeframe *stf_later* are collected in the following tuple set:

```

m.operational_pro_tuples = pyomo.Set(
    within=m.sit*m.pro*m.stf*m.stf,
    initialize=[(sit, pro, stf, stf_later)
        for (sit, pro, stf, stf_later)
        in op_pro_tuples(m.pro_tuples, m)],
    doc='Processes that are still operational through stf_later'
        '(and the relevant years following), if built in stf'
        'in stf.')

```

where the following function is utilized:

```

def op_pro_tuples(pro_tuple, m):
    """ Tuples for operational status of units (processes, transmissions,
    storages) for intertemporal planning.
    Only such tuples where the unit is still operational until the next
    support time frame are valid.
    """
    op_pro = []
    sorted_stf = sorted(list(m.stf))

    for (stf, sit, pro) in pro_tuple:
        for stf_later in sorted_stf:
            index_helper = sorted_stf.index(stf_later)
            if stf_later == max(sorted_stf):
                if (stf_later +
                    m.global_prop.loc[(max(sorted_stf), 'Weight'), 'value
→'] -
                    1 <= stf + m.process_dict['depreciation'][(stf, sit, pro)]):
                    op_pro.append((sit, pro, stf, stf_later))
            elif ((stf_later + sorted_stf[index_helper+1]) / 2 <= stf + m.
→process_dict['depreciation'][(stf, sit, pro)]
                and stf <= stf_later):
                op_pro.append((sit, pro, stf, stf_later))
            else:
                pass

```

(continues on next page)

(continued from previous page)

```
return op_pro
```

Transmissions installed in an earlier support timeframe *stf* and still usable in support timeframe *stf_later* are collected in the following tuple set:

```
m.operational_tra_tuples = pyomo.Set(
    within=m.sit*m.sit*m.tra*m.com*m.stf*m.stf,
    initialize=[(sit, sit_, tra, com, stf, stf_later)
                 for (sit, sit_, tra, com, stf, stf_later)
                 in op_tra_tuples(m.tra_tuples, m)],
    doc='Transmissions that are still operational through stf_later'
        '(and the relevant years following), if built in stf'
        'in stf.')

```

where the following function is utilized:

```
def op_tra_tuples(tra_tuple, m):
    """ s.a. op_pro_tuples """
    op_tra = []
    sorted_stf = sorted(list(m.stf))

    for (stf, sit1, sit2, tra, com) in tra_tuple:
        for stf_later in sorted_stf:
            index_helper = sorted_stf.index(stf_later)
            if stf_later == max(sorted_stf):
                if (stf_later +
                    m.global_prop_dict['value'][(max(sorted_stf), 'Weight
→')] -
                    1 <= stf + m.transmission_dict['depreciation'][(
                        stf, sit1, sit2, tra, com)]):
                    op_tra.append((sit1, sit2, tra, com, stf, stf_later))
            elif (sorted_stf[index_helper + 1] <=
                  stf + m.transmission_dict['depreciation'][(
                      stf, sit1, sit2, tra, com)] and stf <= stf_later):
                op_tra.append((sit1, sit2, tra, com, stf, stf_later))
            else:
                pass

    return op_tra

```

Storages installed in an earlier support timeframe *stf* and still usable in support timeframe *stf_later* are collected in the following tuple set:

```
m.operational_sto_tuples = pyomo.Set(
    within=m.sit*m.sto*m.com*m.stf*m.stf,
    initialize=[(sit, sto, com, stf, stf_later)
                 for (sit, sto, com, stf, stf_later)
                 in op_sto_tuples(m.sto_tuples, m)],
    doc='Processes that are still operational through stf_later'
        '(and the relevant years following), if built in stf'
        'in stf.')

```

where the following function is utilized:

```

def op_sto_tuples(sto_tuple, m):
    """ s.a. op_pro_tuples
    """
    op_sto = []
    sorted_stf = sorted(list(m.stf))

    for (stf, sit, sto, com) in sto_tuple:
        for stf_later in sorted_stf:
            index_helper = sorted_stf.index(stf_later)
            if stf_later == max(sorted_stf):
                if (stf_later +
                    m.global_prop_dict['value'][(max(sorted_stf), 'Weight
→')] -
                    1 <= stf +
                    m.storage_dict['depreciation'][(stf, sit, sto,
→com)]):
                    op_sto.append((sit, sto, com, stf, stf_later))
            elif (sorted_stf[index_helper + 1] <=
                stf +
                m.storage_dict['depreciation'][(stf, sit, sto, com)] and
                stf <= stf_later):
                    op_sto.append((sit, sto, com, stf, stf_later))
            else:
                pass

    return op_sto

```

Variables

All the variables that the optimization model requires to calculate an optimal solution will be listed and defined in this section. A variable is a numerical value that is determined during optimization. Variables can denote a single, independent value, or an array of values. Variables define the search space for optimization. Variables of this optimization model can be separated into sections by their area of use. These Sections are Cost, Commodity, Process, Transmission, Storage and demand side management.

Table 4: Table: Model Variables

Variable	Unit	Description
Cost Variables		
ζ	€	Total System Cost
ζ_{inv}	€	Investment Costs
ζ_{fix}	€	Fix Costs
ζ_{var}	€	Variable Costs
ζ_{fuel}	€	Fuel Costs
ζ_{rev}	€	Revenue Costs
ζ_{pur}	€	Purchase Costs
ζ_{start}	€	Start Costs
Commodity Variables		
ρ_{yvct}	MWh	Stock Commodity Source Term
Q_{yvct}	MWh	Sell Commodity Source Term
ψ_{yvct}	MWh	Buy Commodity Source Term
Process Variables		

Continued on next page

Table 4 – continued from previous page

Variable	Unit	Description
κ_{yvp}	MW	Total Process Capacity
$\hat{\kappa}_{yvp}$	MW	New Process Capacity
β_{yvp}	•	New Process Capacity Units
τ_{yvpt}	MWh	Process Throughput
$\epsilon_{yvcpt}^{\text{in}}$	MWh	Process Input Commodity Flow
$\epsilon_{yvcpt}^{\text{out}}$	MWh	Process Output Commodity Flow
$yvpt$	•	Process On/Off Marker
σ_{yvpt}	•	Process Start-up Marker
Transmission Variables		
κ_{yaf}	MW	Total transmission Capacity
$\hat{\kappa}_{yaf}$	MW	New Transmission Capacity
β_{yaf}	•	New Transmission Capacity Units
π_{yaft}^{in}	MWh	Transmission Input Commodity Flow
π_{yaft}^{out}	MWh	Transmission Output Commodity Flow
DCPF Transmission Variables		
θ_{yvt}	deg.	Voltage Angle
π_{yaft}^{in}	MW	Absolute Transmission Flow
Storage Variables		
κ_{yvs}^c	MWh	Total Storage Size
$\hat{\kappa}_{yvs}^c$	MWh	New Storage Size
β_{yvs}^c	•	New Storage Size Units
κ_{yvs}^p	MW	Total Storage Power
$\hat{\kappa}_{yvs}^p$	MW	New Storage Power
β_{yvs}^c	•	New Storage Power Units
$\epsilon_{yvst}^{\text{in}}$	MWh	Storage Input Commodity Flow
$\epsilon_{yvst}^{\text{out}}$	MWh	Storage Output Commodity Flow
$\epsilon_{yvst}^{\text{con}}$	MWh	Storage Energy Content
Demand Side Management Variables		
$\delta_{yvct}^{\text{up}}$	MWh	DSM Upshift
$\delta_{t,tt,yvc}^{\text{down}}$	MWh	DSM Downshift

Cost Variables

Total System Cost, ζ : the variable ζ represents the *total expense incurred* in reaching the satisfaction of the given energy demand in the entire modeling horizon. If only a fraction of a year is modeled in each support timeframe, the costs are scaled to the annual expenditures. The total cost is calculated by the sum total of all costs by type ($\zeta_r, \forall r \in R$) and defined as `costs` by the following code fragment:

```
m.costs = pyomo.Var(  
    m.cost_type,  
    within=pyomo.Reals,  
    doc='Costs by type (EUR/a)')
```

System costs are divided into the 7 cost types invest, fix, variable, fuel, purchase, sell and environmental. The separation of costs by type, facilitates business planning and provides calculation accuracy. These cost types are hardcoded, which means they are not considered to be fixed or changed by the user.

For more information on the definition of these variables see section [Minimal optimization model](#) and for their implementation see section [Objective function](#).

Commodity Variables

Stock Commodity Source Term, ρ_{yvct} , `e_co_stock`, MWh : The variable ρ_{yvct} represents the energy amount in [MWh] that is being used by the system of commodity c from type stock ($\forall c \in C_{\text{stock}}$) in support timeframe y ($\forall y \in Y$) in a site v ($\forall v \in V$) at timestep t ($\forall t \in T_m$). In script `model.py` this variable is defined by the variable `e_co_stock` and initialized by the following code fragment:

```
m.e_co_stock = pyomo.Var(  
    m.tm, m.com_tuples,  
    within=pyomo.NonNegativeReals,  
    doc='Use of stock commodity source (MWh) at a given timestep')
```

Sell Commodity Source Term, ϱ_{yvct} , `e_co_sell`, MWh : The variable ϱ_{yvct} represents the energy amount in [MWh] that is being used by the system of commodity c from type sell ($\forall c \in C_{\text{sell}}$) in support timeframe y ($\forall y \in Y$) in a site v ($\forall v \in V$) at timestep t ($\forall t \in T_m$). In script `model.py` this variable is defined by the variable `e_co_sell` and initialized by the following code fragment:

```
m.e_co_sell = pyomo.Var(  
    m.tm, m.com_tuples,  
    within=pyomo.NonNegativeReals,  
    doc='Use of sell commodity source (MWh) at a given timestep')
```

Buy Commodity Source Term, ψ_{yvct} , `e_co_buy`, MWh : The variable ψ_{yvct} represents the energy amount in [MWh] that is being used by the system of commodity c from type buy ($\forall c \in C_{\text{buy}}$) in support timeframe y ($\forall y \in Y$) in a site v ($\forall v \in V$) at timestep t ($\forall t \in T_m$). In script `model.py` this variable is defined by the variable `e_co_buy` and initialized by the following code fragment:

```
m.e_co_buy = pyomo.Var(  
    m.tm, m.com_tuples,  
    within=pyomo.NonNegativeReals,  
    doc='Use of buy commodity source (MWh) at a given timestep')
```

Process Variables

Total Process Capacity, κ_{yvp} , `cap_pro`: The variable κ_{yvp} represents the total potential throughput (capacity) of a process tuple p_{yv} ($\forall p \in P, \forall v \in V$, forall y in Y), that is required in the energy system. The total process capacity includes both the already installed process capacity and the additional new process capacity that needs to be installed. Since the costs of the process technologies are mostly directly proportional to the maximum possible output (and correspondingly to the capacity) of processes, this variable acts as a scale factor of process technologies. For further information see **Process Capacity Rule**. This variable is expressed in the unit (MW). In script `model.py` this variable is defined by the model variable `cap_pro` and initialized by the following code fragment:

```
m.cap_pro = pyomo.Var(
    m.pro_tuples,
    within=pyomo.NonNegativeReals,
    doc='Total process capacity (MW)')
```

New Process Capacity, $\hat{\kappa}_{yvp}$, `cap_pro_new`: The variable $\hat{\kappa}_{yvp}$ represents the capacity of a process tuple p_{yv} ($\forall p \in P, \forall v \in V$) that needs to be installed additionally to the energy system in support timeframe y in site v in order to provide the optimal solution. This variable is expressed in the unit MW. In script `model.py` this variable is defined by the model variable `cap_pro_new` and initialized by the following code fragment:

```
m.cap_pro_new = pyomo.Var(
    m.pro_tuples,
    within=pyomo.NonNegativeReals,
    doc='New process capacity (MW)')
```

New Process Capacity Units, β_{yvp} , `pro_cap_unit`: The variable β_{yvp} represents the number of capacity blocks of a process tuple p_{yv} ($\forall p \in P, \forall v \in V$) that needs to be installed additionally to the energy system in support timeframe y in site v in order to provide the optimal solution. In script `model.py` this variable is defined by the model variable `pro_cap_unit` and initialized by the following code fragment:

```
m.pro_cap_unit = pyomo.Var(
    m.pro_tuples,
    within=pyomo.NonNegativeIntegers,
    doc='Number of newly installed capacity units')
```

Process Throughput, τ_{yvp} , `tau_pro`: The variable τ_{yvp} represents the measure of (energetic) activity of a process tuple p_{yv} ($\forall p \in P, \forall v \in V, \forall y \in Y$) at a timestep t ($\forall t \in T_m$). Based on the process throughput amount in a given timestep of a process, flow amounts of the process' input and output commodities at that timestep can be calculated by scaling the process throughput with corresponding process input and output ratios. For further information see **Process Input Ratio** and **Process Output Ratio**. The process throughput variable is expressed in the unit MWh. In script `model.py` this variable is defined by the model variable `tau_pro` and initialized by the following code fragment:

```
m.tau_pro = pyomo.Var(
    m.tm, m.pro_tuples,
    within=pyomo.NonNegativeReals,
    doc='Activity (MWh) through process')
```

Process Input Commodity Flow, $\epsilon_{yvcpt}^{\text{in}}$, `e_pro_in`: The variable $\epsilon_{yvcpt}^{\text{in}}$ represents the commodity input flow into a process tuple p_{yv} ($\forall p \in P, \forall v \in V, \forall y \in Y$) caused by an input commodity c ($\forall c \in C$)

at a timestep t ($\forall t \in T_m$). This variable is generally expressed in the unit MWh. In script `model.py` this variable is defined by the model variable `e_pro_in` and initialized by the following code fragment:

```
m.e_pro_in = pyomo.Var(
    m.tm, m.pro_tuples, m.com,
    within=pyomo.NonNegativeReals,
    doc='Flow of commodity into process at a given timestep')
```

Process Output Commodity Flow, $\epsilon_{yvcpt}^{\text{out}}$, `e_pro_out`: The variable $\epsilon_{yvcpt}^{\text{out}}$ represents the commodity flow output out of a process tuple p_{yv} ($\forall p \in P, \forall v \in V, \forall y \in Y$) caused by an output commodity c ($\forall c \in C$) at a timestep t ($\forall t \in T_m$). This variable is generally expressed in the unit MWh (or tonnes e.g. for the environmental commodity ‘CO2’). In script `model.py` this variable is defined by the model variable `e_pro_out` and initialized by the following code fragment:

```
m.e_pro_out = pyomo.Var(
    m.tm, m.pro_tuples, m.com,
    within=pyomo.NonNegativeReals,
    doc='Flow of commodity out of process at a given timestep')
```

Process On/Off Marker, y_{vpt} , `on_off`: The boolean variable y_{vpt} marks whether process tuple p_{yv} ($\forall p \in P^{\text{on/off}}, \forall v \in V, \forall y \in Y$) is on and producing (y_{vpt} is 1) or it is not producing (y_{vpt} is 0) at a timestep t . While not producing, the process is either turned off or it started, without reaching the minimum fraction P_{yvp} . In the script `AdvancedProcesses.py`, this variable is defined by the model variable `on_off` and initialized by the following code fragment:

```
m.on_off = pyomo.Var(
    m.t, m.pro_on_off_tuples,
    within=pyomo.Boolean,
    doc='Turn on/off a process with minimum working load')
```

Process Start-up Marker, σ_{yvpt} , `start_ups`: The boolean variable σ_{yvpt} marks whether process tuple p_{yv} ($\forall p \in P^{\text{on/off}}, \forall v \in V, \forall y \in Y$) is starting (σ_{yvpt} becomes 1) or not (σ_{yvpt} is 0) at a timestep t . The process is considered to start when its output `e_pro_out` becomes greater than 0. In the script `AdvancedProcesses.py`, this variable is defined by the model variable `start_ups` and initialized by the following code fragment:

```
m.start_up = pyomo.Var(
    m.tm, m.pro_start_up_tuples,
    within=pyomo.Boolean,
    doc='Start-up marker')
```

Transmission Variables

Total Transmission Capacity, κ_{yaf} , `cap_tra`: The variable κ_{yaf} represents the total potential transfer power of a transmission tuple f_{yca} , where a represents the arc from an origin site v_{out} to a destination site v_{in} . The total transmission capacity includes both the already installed transmission capacity and the additional new transmission capacity that needs to be installed. This variable is expressed in the unit MW. In script `transmission.py` this variable is defined by the model variable `cap_tra` and initialized by the following code fragment:

```
m.cap_tra = pyomo.Var(
    m.tra_tuples,
```

(continues on next page)

(continued from previous page)

```
within=pyomo.NonNegativeReals,
doc='Total transmission capacity (MW)')
```

New Transmission Capacity, $\hat{\kappa}_{yaf}$, `cap_tra_new`: The variable $\hat{\kappa}_{yaf}$ represents the additional capacity, that needs to be installed, of a transmission tuple f_{yca} , where a represents the arc from an origin site v_{out} to a destination site v_{in} . This variable is expressed in the unit MW. In script `transmission.py` this variable is defined by the model variable `cap_tra_new` and initialized by the following code fragment:

```
m.cap_tra_new = pyomo.Var(
    m.tra_tuples,
    within=pyomo.NonNegativeReals,
    doc='New transmission capacity (MW)')
```

New Transmission Capacity Units, β_{yaf} , `tra_cap_unit`: The variable β_{yaf} represents the number of additional capacity blocks of a transmission tuple f_{yca} that need to be installed, where a represents the arc from an origin site v_{out} to a destination site v_{in} . In script `transmission.py` this variable is defined by the model variable `cap_tra_new` and initialized by the following code fragment:

```
m.tra_cap_unit = pyomo.Var(
    m.tra_block_tuples,
    within=pyomo.NonNegativeIntegers,
    doc='New transmission capacity blocks')
```

Transmission Input Commodity Flow, π_{yaft}^{in} , `e_tra_in`: The variable π_{yaft}^{in} represents the commodity flow input into a transmission tuple f_{yca} at a timestep t , where a represents the arc from an origin site v_{out} to a destination site v_{in} . This variable is expressed in the unit MWh. In script `urbs.py` this variable is defined by the model variable `e_tra_in` and initialized by the following code fragment:

```
m.e_tra_in = pyomo.Var(
    m.tm, m.tra_tuples,
    within=pyomo.NonNegativeReals,
    doc='Commodity flow into transmission line (MWh) at a given timestep')
```

Transmission Output Commodity Flow, π_{yaft}^{out} , `e_tra_out`: The variable π_{yaft}^{out} represents the commodity flow output out of a transmission tuple f_{ca} at a timestep t , where a represents the arc from an origin site v_{out} to a destination site v_{in} . This variable is expressed in the unit MWh. In script `urbs.py` this variable is defined by the model variable `e_tra_out` and initialized by the following code fragment:

```
m.e_tra_out = pyomo.Var(
    m.tm, m.tra_tuples,
    within=pyomo.NonNegativeReals,
    doc='Power flow out of transmission line (MWh) at a given timestep')
```

DCPF Transmission Variables

If the DC Power Flow transmission modelling is activated, two new variables are introduced to the model.

Voltage Angle, θ_{yvt} , `voltage_angle`: The variable θ_{yvt} represents the voltage angle of a site v , which has a DCPF transmission line connection, at a timestep t . This variable is expressed in the unit

degrees. In script `urbs.py` this variable is defined by the model variable `voltage_angle` and initialized by the following code fragment:

```
m.voltage_angle = pyomo.Var(
    m.tm, m.stf, m.sit,
    within=pyomo.Reals,
    doc='Voltage angle of a site')
```

Absolute Value of Transmission Commodity Flow, π_{yaft}^{in} , `e_tra_abs`: The variable π_{yaft}^{in} represents the absolute value of the transmission commodity flow on a DCPF transmission tuple f_{yca} at a timestep t , where a represents the arc from an origin site v_{out} to a destination site v_{in} . This variable is expressed in the unit MWh. In script `urbs.py` this variable is defined by the model variable `e_tra_abs` and initialized by the following code fragment:

```
m.e_tra_abs = pyomo.Var(
    m.tm, m.tra_tuples_dc,
    within=pyomo.NonNegativeReals,
    doc='Absolute power flow on transmission line (MW) per timestep')
```

Transmission Commodity Flow Domain Changes : DC Power Flow transmission lines are represented by bidirectional single arcs instead of unidirectional symmetrical arcs as in the default transmission model. Consequently the power flow is allowed to be both positive or negative for DCPF transmission lines contrary to the transport transmission lines. For this reason, the domains of the variables transmission input commodity flow π_{yaft}^{in} and transmission output commodity flow π_{yaft}^{out} are defined with the `e_tra_domain_rule()` function depending on the corresponding transmission tuple set. These variables are defined by the model variables `e_tra_in` and `e_tra_out` and intialized by the code fragment:

```
m.e_tra_in = pyomo.Var(
    m.tm, m.tra_tuples,
    within=e_tra_domain_rule,
    doc='Power flow into transmission line (MW) per timestep')
m.e_tra_out = pyomo.Var(
    m.tm, m.tra_tuples,
    within=e_tra_domain_rule,
    doc='Power flow out of transmission line (MW) per timestep')
```

The function `e_tra_domain_rule()` is given by the code fragment:

```
def e_tra_domain_rule(m, tm, stf, sin, sout, tra, com):
    # assigning e_tra_in and e_tra_out variable domains for transport and_
    ↪DCPF
    if (stf, sin, sout, tra, com) in m.tra_tuples_dc:
        return pyomo.Reals
    elif (stf, sin, sout, tra, com) in m.tra_tuples_tp:
        return pyomo.NonNegativeReals
```

Storage Variables

Total Storage Size, κ_{yvs}^c , `cap_sto_c`: The variable κ_{yvs}^c represents the total load capacity of a storage tuple s_{yvc} . The total storage load capacity includes both the already installed storage load capacity and the additional new storage load capacity that needs to be installed. This variable is expressed in unit MWh. In script `model.py` this variable is defined by the model variable `cap_sto_c` and initialized by the following code fragment:

```
m.cap_sto_c = pyomo.Var(
    m.sto_tuples,
    within=pyomo.NonNegativeReals,
    doc='Total storage size (MWh)')
```

New Storage Size, $\hat{\kappa}_{yvs}^c$, cap_sto_c_new: The variable $\hat{\kappa}_{yvs}^c$ represents the additional storage load capacity of a storage tuple s_{vc} that needs to be installed to the energy system in order to provide the optimal solution. This variable is expressed in the unit MWh. In script `model.py` this variable is defined by the model variable `cap_sto_c_new` and initialized by the following code fragment:

```
m.cap_sto_c_new = pyomo.Var(
    m.sto_tuples,
    within=pyomo.NonNegativeReals,
    doc='New storage size (MWh)')
```

New Storage Size Units, β_{yvs}^c , sto_cap_c_unit: The variable $\hat{\kappa}_{yvs}^c$ represents the number of additional storage load capacity blocks of a storage tuple s_{vc} that needs to be installed to the energy system in order to provide the optimal solution. In script `storage.py` this variable is defined by the model variable `cap_sto_c_unit` and initialized by the following code fragment:

```
m.sto_cap_c_unit = pyomo.Var(
    m.sto_block_c_tuples,
    within=pyomo.NonNegativeIntegers,
    doc='New storage size units')
```

Total Storage Power, κ_{yvs}^p , cap_sto_p: The variable κ_{yvs}^p represents the total potential discharge power of a storage tuple s_{vc} . The total storage power includes both the already installed storage power and the additional new storage power that needs to be installed. This variable is expressed in the unit MW. In script `model.py` this variable is defined by the model variable `cap_sto_p` and initialized by the following code fragment:

```
m.cap_sto_p = pyomo.Var(
    m.sto_tuples,
    within=pyomo.NonNegativeReals,
    doc='Total storage power (MW)')
```

New Storage Power, $\hat{\kappa}_{yvs}^p$, cap_sto_p_new: The variable $\hat{\kappa}_{yvs}^p$ represents the additional potential discharge power of a storage tuple s_{vc} that needs to be installed to the energy system in order to provide the optimal solution. This variable is expressed in the unit MW. In script `model.py` this variable is defined by the model variable `cap_sto_p_new` and initialized by the following code fragment:

```
m.cap_sto_p_new = pyomo.Var(
    m.sto_tuples,
    within=pyomo.NonNegativeReals,
    doc='New storage power (MW)')
```

New Storage Power Units, β_{yvs}^c , sto_cap_p_unit: The variable β_{yvs}^c represents the number of additional potential discharge power blocks of a storage tuple s_{vc} that needs to be installed to the energy system in order to provide the optimal solution. In the script `storage.py` this variable is defined by the model variable `sto_cap_p_unit` and initialized by the following code fragment:

```
m.sto_cap_p_unit = pyomo.Var(
    m.sto_block_p_tuples,
```

(continues on next page)

(continued from previous page)

```
within=pyomo.NonNegativeIntegers,
doc='New storage power units')
```

Storage Input Commodity Flow, $\epsilon_{yvc}^{\text{in}}$, `e_sto_in`: The variable $\epsilon_{yvc}^{\text{in}}$ represents the input commodity flow into a storage tuple s_{yvc} at a timestep t . Input commodity flow into a storage tuple can also be defined as the charge of a storage tuple. This variable is expressed in the unit MWh. In `script model.py` this variable is defined by the model variable `e_sto_in` and initialized by the following code fragment:

```
m.e_sto_in = pyomo.Var(
    m.tm, m.sto_tuples,
    within=pyomo.NonNegativeReals,
    doc='Commodity flow into storage (MWh) at a given timestep')
```

Storage Output Commodity Flow, $\epsilon_{yvc}^{\text{out}}$, `e_sto_out`: The variable $\epsilon_{yvc}^{\text{out}}$ represents the output commodity flow out of a storage tuple s_{yvc} at a timestep t . Output commodity flow out of a storage tuple can also be defined as the discharge of a storage tuple. This variable is expressed in the unit MWh. In `script model.py` this variable is defined by the model variable `e_sto_out` and initialized by the following code fragment:

```
m.e_sto_out = pyomo.Var(
    m.tm, m.sto_tuples,
    within=pyomo.NonNegativeReals,
    doc='Commodity flow out of storage (MWh) at a given timestep')
```

Storage Energy Content, $\epsilon_{yvc}^{\text{con}}$, `e_sto_con`: The variable $\epsilon_{yvc}^{\text{con}}$ represents the energy amount that is loaded in a storage tuple s_{yvc} at a timestep t . This variable is expressed in the unit MWh. In `script urbs.py` this variable is defined by the model variable `e_sto_out` and initialized by the following code fragment:

```
m.e_sto_con = pyomo.Var(
    m.t, m.sto_tuples,
    within=pyomo.NonNegativeReals,
    doc='Energy content of storage (MWh) at a given timestep')
```

Demand Side Management Variables

DSM Upshift, δ_{yvc}^{up} , `dsm_up`, MWh: The variable δ_{yvc}^{up} represents the DSM upshift in time step t in support timeframe y in site v for commodity c . It is only defined for all `dsm_site_tuples`. The following code fragment shows the definition of the variable:

```
m.dsm_up = pyomo.Var(
    m.tm, m.dsm_site_tuples,
    within=pyomo.NonNegativeReals,
    doc='DSM upshift (MWh) of a demand commodity at a given timestep')
```

DSM Downshift, $\delta_{t,tt,yvc}^{\text{down}}$, `dsm_down`, MWh: The variable $\delta_{t,tt,yvc}^{\text{down}}$ represents the DSM downshift in timestep tt caused by the upshift in time t in support timeframe y in site v for commodity c . The special combinations of timesteps t and tt for each (support timeframe, site, commodity) combination is created by the `dsm_down_tuples`. The definition of the variable is shown in the code fragment:


```
m.dsm_down = pyomo.Var(
m.dsm_down_tuples,
within=pyomo.NonNegativeReals,
doc='DSM downshift (MWh) of a demand commodity at a given timestep')
```

Parameters

All the parameters that the optimization model requires to calculate an optimal solution will be listed and defined in this section. A parameter is a datapoint, that is provided by the user before the optimization simulation starts. These parameters are the values that define the specifications of the modelled energy system. Parameters of this optimization model can be separated into two main parts, these are Technical and Economical Parameters.

Technical Parameters

Table 5: Table: Technical Model Parameters

Parameter	Unit	Description
General Technical Parameters		
w	–	Fraction of 1 year of modeled timesteps
Δt	h	Timestep Size
W	a	Weight of last support timeframe
Commodity Technical Parameters		
d_{yvct}	MWh	Demand for Commodity
s_{yvct}	–	Intermittent Supply Capacity Factor
\bar{l}_{yvc}	MW	Maximum Stock Supply Limit Per Hour
\bar{L}_{yvc}	MWh	Maximum Annual Stock Supply Limit Per Vertex
\bar{m}_{yvc}	t/h	Maximum Environmental Output Per Hour
\bar{M}_{yvc}	t	Maximum Annual Environmental Output
\bar{g}_{yvc}	MW	Maximum Sell Limit Per Hour
\bar{G}_{yvc}	MWh	Maximum Annual Sell Limit
\bar{b}_{yvc}	MW	Maximum Buy Limit Per Hour
\bar{B}_{yvc}	MWh	Maximum Annual Buy Limit
$\bar{L}_{CO_2,y}$	t	Maximum Global Annual CO2 Emission Limit
$\bar{\bar{L}}_{CO_2}$	t	CO2 Emission Budget for modeling horizon
Process Technical Parameters		
K_{yvp}	MW	Process Capacity Lower Bound
K_{vp}	MW	Process Capacity Installed
K_{yvp}	MW	Process Capacity Upper Bound
T_{vp}	MW	Remaining lifetime of installed processes
\overline{PG}_{yvp}^{up}	1/h	Process Maximal Power Ramp Up Gradient (relat
$\overline{PG}_{yvp}^{down}$	1/h	Process Maximal Power Ramp Down Gradient (re
\overline{ST}_{yvp}	h	Process Starting Time
\overline{SR}_{yvp}	1/h	Process Starting Ramp
\underline{P}_{yvp}	–	Process Minimum Part Load Fraction
f_{yvp}^{out}	–	Process Output Ratio multiplier
r_{ypc}^{in}	–	Process Input Ratio

Continued on next page

Table 5 – continued from previous page

Parameter	Unit	Description
r_{ypc}^{in}	–	Process Partial Input Ratio
r_{ypc}^{out}	–	Process Partial Output Ratio
r_{ypc}^{out}	–	Process Output Ratio
K_{yvp}^{block}	MW	Process New Capacity Block
Storage Technical Parameters		
I_{yvs}	–	Initial and Final State of Charge
e_{yvs}^{in}	–	Storage Efficiency During Charge
e_{yvs}^{out}	–	Storage Efficiency During Discharge
d_{yvs}	1/h	Storage Self-discharge Per Hour
\underline{K}_{yvs}^c	MWh	Storage Capacity Lower Bound
\overline{K}_{yvs}^c	MWh	Storage Capacity Installed
\underline{K}_{yvs}^p	MW	Storage Capacity Upper Bound
\overline{K}_{yvs}^p	MW	Storage Power Lower Bound
\underline{K}_{yvs}^p	MW	Storage Power Installed
\overline{K}_{yvs}^p	MW	Storage Power Upper Bound
T_{vs}	MW	Remaining lifetime of installed storages
$k_{yvs}^{E/P}$	h	Storage Energy to Power Ratio
$K_{yvs}^{c,block}$	MWh	Storage New Capacity Block
$K_{yvs}^{p,block}$	MW	Storage New Power Block
Transmission Technical Parameters		
e_{yaf}	–	Transmission Efficiency
\underline{K}_{yaf}	MW	Transmission Capacity Lower Bound
\overline{K}_{yaf}	MW	Transmission Capacity Installed
\underline{K}_{yaf}	MW	Transmission Capacity Upper Bound
T_{af}	year	Remaining lifetime of installed transmission
K_{yaf}^{block}	MW	Transmission New Capacity Block
DCPF Transmission Technical Parameters		
X_{yaf}	p.u	Transmission Reactance
dl_{yaf}	deg.	Voltage Angle Difference Limit
$V_{yafbase}$	kV	Transmission Base Voltage
K_{yaf}^{block}	–	Transmission New Capacity Block
Demand Side Management Parameters		
e_{yvc}	–	DSM Efficiency
y_{yvc}	–	DSM Delay Time
o_{yvc}	–	DSM Recovery Time
\overline{K}_{yvc}^{up}	MW	DSM Maximal Upshift Per Hour
$\overline{K}_{yvc}^{down}$	MW	DSM Maximal Downshift Per Hour

General Technical Parameters

Weight, w , weight: The parameter w helps to scale variable costs and emissions from the length of simulation, that the energy system model is being observed, to an annual result. This parameter represents the fraction of a year (8760 hours) of the observed time span. The observed time span is calculated by the product of number of time steps of the set T and the time step duration. In script `model.py` this parameter is defined by the model parameter `weight` and initialized by the following code fragment:

```
m.weight = pyomo.Param(
    initialize=float(8760) / (len(m.tm) * dt),
    doc='Pre-factor for variable costs and emissions for an annual result')
```

Timestep Duration, Δt , dt: The parameter Δt represents the duration between two sequential timesteps t_x and t_{x+1} . This is calculated by the subtraction of smaller one from the bigger of the two sequential timesteps $\Delta t = t_{x+1} - t_x$. This parameter is the unit of time for the optimization model, is expressed in the unit h and by default the value is set to 1. In script `model.py` this parameter is defined by the model parameter `dt` and initialized by the following code fragment:

```
m.dt = pyomo.Param(
    initialize=dt,
    doc='Time step duration (in hours), default: 1')
```

The user can set the parameter in script `runme.py` in the line:

```
dt = 1 # length of each time step (unit: hours)
```

Weight of last modeled support timeframe, W , `m.global_prop.loc[(min(m.stf), 'Cost budget'), 'value']`: This parameter specifies how long the time interval represented by the last support timeframe is. The unit of this parameter is years. By extension it also specifies the end of the modeling horizon. The parameter is set in the spreadsheet corresponding to the last support timeframe in worksheet “Global” in the line denoted “Weight” in the column titled “value”.

Commodity Technical Parameters

Demand for Commodity, d_{yvc} , `m.demand_dict[(stf, sit, com)][tm]`: The parameter represents the energy amount of a demand commodity tuple c_{yvq} required at a timestep t ($\forall y \in Y, \forall v \in V, q = \text{Demand}, \forall t \in T_m$). The unit of this parameter is MWh. This data is to be provided by the user and to be entered in the spreadsheet corresponding to the specified support timeframe. The related section for this parameter in the spreadsheet can be found in the “Demand” sheet. Here each row represents another timestep t and each column represent a commodity tuple c_{yvq} . Rows are named after the timestep number n of timesteps t_n . Columns are named after the combination of site name v and commodity name c respecting the order and separated by a period(.). For example (Mid, Elec) represents the commodity Elec in site Mid. Commodity Type q is omitted in column declarations, because every commodity of this parameter has to be from commodity type *Demand* in any case.

Intermittent Supply Capacity Factor, s_{yvc} , `m.supim_dict[(stf, sit, coin)][tm]`: The parameter s_{yvc} represents the normalized availability of a supply intermittent commodity c ($\forall c \in C_{\text{sup}}$) in a support timeframe y and site v at a timestep t . In other words this parameter gives the ratio of current available energy amount to maximum potential energy amount of a supply intermittent commodity. This data is to be provided by the user and to be entered in the spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under the “SupIm” sheet. Here each row represents another timestep t and each column represent a commodity tuple c_{vq} . Rows are named after the timestep number n of timesteps t_n . Columns are named after the combination of site name v and commodity name c , in this respective order and separated by a period(.). For example (Mid.Elec) represents the commodity Elec in site Mid. Commodity Type q is omitted in column declarations, because every commodity of this parameter has to be from commodity type *SupIm* in any case.

Maximum Stock Supply Limit Per Hour, \bar{l}_{yvc} , `m.commodity_dict['maxperhour'][(stf, sit, com, com_type)]`: The parameter \bar{l}_{yvc} represents the maximum energy amount of a stock

commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = "Stock"$) that energy model is allowed to use per hour. The unit of this parameter is MW. This parameter applies to every timestep and does not vary for each timestep t . This parameter is to be provided by the user and to be entered in spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under the `Commodity` sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “maxperhour” represents the parameter \bar{l}_{yvc} . If there is no desired restriction of a stock commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Annual Stock Supply Limit Per Vertex, \bar{L}_{yvc} , `m.commodity_dict['max'][(stf, sit, com, com_type)]`: The parameter \bar{L}_{yvc} represents the maximum energy amount of a stock commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = "Stock"$) that energy model is allowed to use annually. The unit of this parameter is MWh. This parameter is to be provided by the user and to be entered in spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under the `Commodity` sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “max” represents the parameter \bar{L}_{yvc} . If there is no desired restriction of a stock commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Environmental Output Per Hour, \bar{m}_{yvc} , `m.commodity_dict['maxperhour'][(stf, sit, com, com_type)]`: The parameter \bar{m}_{yvc} represents the maximum energy amount of an environmental commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = "Env"$) that energy model is allowed to produce and release to environment per time step. This parameter applies to every timestep and does not vary for each timestep t/h . This parameter is to be provided by the user and to be entered in spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under the `Commodity` sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “maxperhour” represents the parameter \bar{m}_{yvc} . If there is no desired restriction of an environmental commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Annual Environmental Output, \bar{M}_{yvc} , `m.commodity_dict['max'][(stf, sit, com, com_type)]`: The parameter \bar{M}_{yvc} represents the maximum energy amount of an environmental commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = "Env"$) that energy model is allowed to produce and release to environment annually. This parameter is to be provided by the user and to be entered in spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under the `Commodity` sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “max” represents the parameter \bar{M}_{yvc} . If there is no desired restriction of a stock commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Sell Limit Per Hour, \bar{g}_{yvc} , `m.commodity_dict['maxperhour'][(stf, sit, com, com_type)]`: The parameter \bar{g}_{yvc} represents the maximum energy amount of a sell commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = "Sell"$) that energy model is allowed to sell per hour. The unit of this parameter is MW. This parameter applies to every timestep and does not vary for each timestep t . This parameter is to be provided by the user and to be entered in spreadsheet. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the `Commodity` sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “maxperhour” represents the parameter \bar{g}_{yvc} . If there is no desired restriction of a sell commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Annual Sell Limit, \bar{G}_{yvc} , `m.commodity_dict['max'][(stf, sit, com, com_type)]`: The parameter \bar{G}_{yvc} represents the maximum energy amount of a sell commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = "Sell"$) that energy model is allowed to sell annually. The unit of this parameter is MWh. This parameter is to be provided by the user and to be entered in spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under

the Commodity sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “max” represents the parameter \bar{G}_{yvc} . If there is no desired restriction of a sell commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Buy Limit Per Hour, \bar{b}_{yvc} , `m.commodity_dict['maxperhour'][(stf, sit, com, com_type)]`: The parameter \bar{b}_{yvc} represents the maximum energy amount of a buy commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = \text{"Buy"}$) that energy model is allowed to buy per hour. The unit of this parameter is MW. This parameter applies to every timestep and does not vary for each timestep t . This parameter is to be provided by the user and to be entered in spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under the Commodity sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “maxperhour” represents the parameter \bar{b}_{yvc} . If there is no desired restriction of a sell commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Annual Buy Limit, \bar{B}_{yvc} , `m.commodity_dict['max'][(stf, sit, com, com_type)]`: The parameter \bar{B}_{yvc} represents the maximum energy amount of a buy commodity tuple c_{yvq} ($\forall y \in Y, \forall v \in V, q = \text{"Buy"}$) that energy model is allowed to buy annually. The unit of this parameter is MWh. This parameter is to be provided by the user and to be entered in spreadsheet corresponding to the support timeframe. The related section for this parameter in the spreadsheet can be found under the Commodity sheet. Here each row represents another commodity tuple c_{yvq} and the column with the header label “max” represents the parameter \bar{B}_{yvc} . If there is no desired restriction of a buy commodity tuple usage per timestep, the corresponding cell can be set to “inf” to ignore this parameter.

Maximum Global Annual CO₂ Annual Emission Limit, $\bar{L}_{CO_2,y}$, `m.global_prop.loc[stf, 'CO2 limit']['value']`: The parameter $\bar{L}_{CO_2,y}$ represents the maximum total amount of CO₂ the energy model is allowed to produce and release to the environment annually. If the user desires to set a maximum annual limit to total CO₂ emission across all sites of the energy model in a given support timeframe y , this can be done by entering the desired value to the spreadsheet corresponding to the support timeframe. The related section for this parameter can be found under the sheet “Global”. Here the the cell where the “CO₂ limit” row and “value” column intersects stands for the parameter $\bar{L}_{CO_2,y}$. If the user wants to disable this parameter and restriction it provides, this cell can be set to “inf” or simply be deleted.

CO₂ `‘**emissionbudget**TotalEmissionbudget**,:math :overline{\overline{L}}_{CO_2}`, `m.global_prop.loc[min(m.stf), 'CO2 budget']['value']`: The parameter $\bar{\bar{L}}_{CO_2}$ represents the maximum total amount of CO₂ the energy model is allowed to produce and release to the environment over the entire modeling horizon. If the user desires to set a limit to total CO₂ emission across all sites and the entire modeling horizon of the energy model, this can be done by entering the desired value to the spreadsheet of the first support timeframe. The related section for this parameter can be found under the sheet “Global”. Here the the cell where the “CO₂ budget” row and “value” column intersects stands for the parameter $\bar{\bar{L}}_{CO_2}$. If the user wants to disable this parameter and restriction it provides, this cell can be set to “inf” or simply be deleted.

Process Technical Parameters

Process Capacity Lower Bound, \underline{K}_{yvp} , `m.process_dict['cap-lo'][(stf, sit, pro)]`: The parameter \underline{K}_{yvp} represents the minimum amount of power output capacity of a process p at a site v in support timeframe y , that energy model is required to have. The unit of this parameter is MW. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “cap-lo” represents the parameters \underline{K}_{yvp} belonging to the corresponding process p

and site v combinations. If there is no desired minimum limit for the process capacities, this parameter can be simply set to “0”.

Process Capacity Installed, K_{vp} , `m.process_dict['inst-cap'][(stf, sit, pro)]`: The parameter K_{vp} represents the amount of power output capacity of a process p in a site v , that is already installed to the energy system at the beginning of the modeling period. The unit of this parameter is MW. The related section for this parameter can be found in the spreadsheet corresponding to the first support timeframe under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “inst-cap” represents the parameters K_{vp} belonging to the corresponding process p and site v combinations.

Process Capacity Upper Bound, \bar{K}_{yvp} , `m.process_dict['cap-up'][(stf, sit, pro)]`: The parameter \bar{K}_{yvp} represents the maximum amount of power output capacity of a process p at a site v in support timeframe y , that energy model is allowed to have. The unit of this parameter is MW. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “cap-up” represents the parameters \bar{K}_{yvp} of the corresponding process p and site v combinations. Alternatively, \bar{K}_{yvp} is determined by the column with the label “area-per-cap”, whenever the value in “cap-up” times the value “area-per-cap” is larger than the value in column “area” in sheet “Site” for site v in support timeframe y . If there is no desired maximum limit for the process capacities, both input parameters can be simply set to “inf”.

Remaining lifetime of installed processes, T_{vp} , `m.process.loc[(min(m.stf), sit, pro), 'lifetime']`: The parameter T_{vp} represents the remaining lifetime of already installed units. It is used to determine the set $m.inst_pro_tuples$, i.e. to identify for which support timeframes the installed unit can still be used.

Process Maximal Power Ramp Up Gradient, \overline{PG}_{yvp}^{up} , `m.process_dict['ramp-up-grad'][(stf, sit, pro)]`: The parameter \overline{PG}_{yvp}^{up} represents the maximal power ramp up gradient of a process p at a site v in support timeframe y , that energy model is allowed to have. The unit of this parameter is 1/h. The related section for this parameter in the spreadsheet can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “ramp-up-grad” represents the parameters \overline{PG}_{yvp}^{up} of the corresponding process p and site v combinations. If there is no desired maximum limit for the process power ramp up gradient, this parameter can be simply set to a value larger or equal to 1.

Process Maximal Power Ramp Down Gradient, $\overline{PG}_{yvp}^{down}$, `m.process_dict['ramp-down-grad'][(stf, sit, pro)]`: The parameter $\overline{PG}_{yvp}^{down}$ represents the maximal power ramp down gradient of a process p at a site v in support timeframe y , that energy model is allowed to have. The unit of this parameter is 1/h. The related section for this parameter in the spreadsheet can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “ramp-down-grad” represents the parameters $\overline{PG}_{yvp}^{down}$ of the corresponding process p and site v combinations. If there is no desired maximum limit for the process power ramp down gradient, this parameter can be simply set to a value larger or equal to 1.

Process Starting Time, \overline{ST}_{yvp} , `m.process_dict['start-time'][(stf, sit, pro)]`: The parameter \overline{ST}_{yvp} represents the time required by a process p at a site v in support timeframe y to start. The unit of this parameter is h. The related section for this parameter in the spreadsheet can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “start-time” represents the parameters \overline{ST}_{yvp} of the corresponding process p and site v combinations.

Process Starting Ramp, \overline{SR}_{yvp} : The parameter \overline{SR}_{yvp} represents the ramp of a process p at a site v in

support timeframe y while starting. The unit of this parameter is 1/h. This parameter is not declared directly in the input, being only a derived parameter, calculated as the ratio between the process minimum part load fraction \underline{P}_{yvp} and the process starting time ST_{yvp} .

Process Minimum Part Load Fraction, \underline{P}_{yvp} , $m.process_dict['min-fraction'][(stf, sit, pro)]$: The parameter \underline{P}_{yvp} represents the minimum allowable part load of a process p at a site v in support timeframe y as a fraction of the total process capacity. The related section for this parameter in the spreadsheet can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “min-fraction” represents the parameters \underline{P}_{yvp} of the corresponding process p and site v combinations. The minimum part load fraction parameter constraints is only relevant when the part load behavior for the process is active, i.e., when in the process commodity sheet a value for “ratio-min” is set for at least one input commodity.

Process Output Ratio multiplier, f_{yvpt}^{out} , $m.eff_factor_dict[(stf, sit, pro)]$: The parameter time series f_{yvpt}^{out} allows for a time dependent modification of process outputs and by extension of the efficiency of a process p in site v and support timeframe y . It can be used, e.g., to model temperature dependent efficiencies of processes or to include scheduled maintenance intervals. In the spreadsheet corresponding to the support timeframe this timeseries is set in worksheet “TimeVarEff”. Here each row represents another timestep t and each column represent a process tuple p_{yv} . Rows are named after the timestep number n of timesteps t_n . Columns are named after the combination of site name v and commodity name and process name p respecting the order and separated by a period(.). For example (Mid, Lignite plant) represents the process Lignite plant in site Mid. Note that the output of environmental commodity outputs are not manipulated by this factor as it is typically linked to an input commodity as , e.g., CO2 output is linked to a fossil input.

Process Input Ratio, r_{ypc}^{in} , $m.r_in_dict[(stf, pro, co)]$: The parameter r_{ypc}^{in} represents the ratio of the input amount of a commodity c in a process p and support timeframe y , relative to the process throughput at a given timestep. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Process-Commodity” sheet. Here each row represents another commodity c that either goes in to or comes out of a process p . The column with the header label “ratio” represents the parameters r_{ypc}^{in} of the corresponding process p and commodity c if the latter is an input commodity.

Process Partial Input Ratio, \underline{r}_{ypc}^{in} , $m.r_in_min_fraction[stf, pro, coin]$: The parameter \underline{r}_{ypc}^{in} represents the ratio of the amount of input commodity c a process p and support timeframe y consumes if it is at its minimum allowable partial operation. More precisely, when its throughput τ_{yvpt} has the minimum value $\kappa_{yvp}\underline{P}_{yvp}$. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Process-Commodity” sheet. Here each row represents another commodity c that either goes in to or comes out of a process p . The column with the header label “ratio-min” represents the parameters $\underline{r}_{ypc}^{in,out}$ of the corresponding process p and commodity c if the latter is an input commodity.

Process Output Ratio, r_{ypc}^{out} , $m.r_out_dict[(stf, pro, co)]$: The parameter r_{ypc}^{out} represents the ratio of the output amount of a commodity c in a process p in support timeframe y , relative to the process throughput at a given timestep. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Process-Commodity” sheet. Here each row represents another commodity c that either goes in to or comes out of a process p . The column with the header label “ratio” represents the parameters of the corresponding process p and commodity c if the latter is an output commodity.

Process Partial Output Ratio, $\underline{r}_{ypc}^{out}$, $m.r_out_min_fraction[stf, pro, coo]$: The parameter $\underline{r}_{ypc}^{out}$ represents the ratio of the amount of output commodity c a process p and support timeframe y emits if it is at its minimum allowable partial operation. More precisely, when its throughput τ_{yvpt} has the minimum value $\kappa_{yvp}\underline{P}_{yvp}$. The related section for this parameter in the spreadsheet corresponding

to the support timeframe can be found under the “Process-Commodity” sheet. Here each row represents another commodity c that either goes in to or comes out of a process p . The column with the header label “ratio-min” represents the parameters $L_{ypc}^{\text{in,out}}$ of the corresponding process p and commodity c if the latter is an output commodity.

Process input and output ratios are, in general, used for unit conversion between the different commodities.

Since all costs and capacity constraints take the process throughput τ_{yvp} as the reference, it is reasonable to assign an in- or output ratio of “1” to at least one commodity. The flow of this commodity then tracks the throughput and can be used as a reference. All other values of in- and output ratios can then be adjusted by scaling them by an appropriate factor to the reference commodity flow.

Process New Capacity Block, K_{yvp}^{block} , `m.process_dict['cap-block'][(stf, sit, pro)]`: The parameter K_{yvp}^{block} represents the capacity of all newly installed units of a process p at a site v in the support timeframe y . The unit of this parameter is MW. The related section for this parameter in the spreadsheet can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “cap-block” represents the parameters K_{yvp}^{block} of the corresponding process p and site v combinations.

Storage Technical Parameters

Initial and Final State of Charge (relative), I_{yvs} , `m.storage_dict['init'][(stf, sit, sto, com)]`: The parameter I_{yvs} represents the initial state of charge of a storage s in a site v and support timeframe y . If this value is left unspecified, the initial state of charge is variable. The initial and final value are set as identical in each modeled support timeframe to avoid windfall profits through emptying of a storage. The value of this parameter is expressed as a normalized percentage, where “1” represents a fully loaded storage and “0” represents an empty storage. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “init” represents the parameters for corresponding storage s , site v , commodity c combinations. When no initial value is to be set this cell can be left empty.

Storage Efficiency During Charge, e_{yvs}^{in} , `m.storage_dict['eff-in'][(stf, sit, sto, com)]`: The parameter e_{yvs}^{in} represents the charging efficiency of a storage s in a site v and support timeframe y that stores a commodity c . The charging efficiency shows, how much of a desired energy and accordingly power can be successfully stored into a storage. The value of this parameter is expressed as a normalized percentage, where “1” represents a charging without energy losses. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “eff-in” represents the parameters e_{yvs}^{in} for corresponding storage tuples.

Storage Efficiency During discharge, e_{yvs}^{out} , `m.storage_dict['eff-out'][(stf, sit, sto, com)]`: The parameter e_{yvs}^{out} represents the discharging efficiency of a storage s in a site v and support timeframe y that stores a commodity c . The discharging efficiency shows, how much of a desired energy and accordingly power can be successfully released from a storage. The value of this parameter is expressed as a normalized percentage, where “1” represents a discharging without energy losses. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “eff-out” represents the parameters e_{yvs}^{out} for corresponding storage tuples.

Storage Self-discharge Per Hour, d_{yvs} , `m.storage_dict['discharge'][(stf, sit, sto, com)]`: The parameter d_{yvs} represents the fraction of the energy content within a storage which is lost due to self-discharge per hour. It introduces an exponential decay of a given storage state if no charging/discharging takes place. The unit of this parameter is 1/h. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “discharge” represents the parameters d_{yvs} for corresponding storage tuples.

Storage Capacity Lower Bound, \underline{K}_{yvs}^c , `m.storage_dict['cap-lo-c'][(stf, sit, sto, com)]`: The parameter \underline{K}_{yvs}^c represents the minimum amount of energy content capacity required for a storage s storing a commodity c in a site v in support timeframe y . The unit of this parameter is MWh. The related section for this parameter in the spreadsheet can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “cap-lo-c” represents the parameters \underline{K}_{yvs}^c for corresponding storage tuples. If there is no desired minimum limit for the storage energy content capacities, this parameter can be simply set to “0”.

Storage Capacity Installed, K_{vs}^c , `m.storage_dict['inst-cap-c'][(min(m.stf), sit, sto, com)]`: The parameter K_{vs}^c represents the amount of energy content capacity of a storage s storing commodity c in a site v and support timeframe y , that is already installed to the energy system at the beginning of the model horizon. The unit of this parameter is MWh. The related section for this parameter in the spreadsheet corresponding to the first support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “inst-cap-c” represents the parameters K_{vs}^c for corresponding storage tuples.

Storage Capacity Upper Bound, \overline{K}_{yvs}^c , `m.storage_dict['cap-up-c'][(stf, sit, sto, com)]`: The parameter \overline{K}_{yvs}^c represents the maximum amount of energy content capacity allowed of a storage s storing a commodity c in a site v in support timeframe y . The unit of this parameter is MWh. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “cap-up-c” represents the parameters \overline{K}_{yvs}^c for corresponding storage tuples. If there is no desired maximum limit for the storage energy content capacities, this parameter can be simply set to “inf”.

Storage Power Lower Bound, \underline{K}_{yvs}^p , `m.storage_dict['cap-lo-p'][(stf, sit, sto, com)]`: The parameter \underline{K}_{yvs}^p represents the minimum amount of charging/discharging power required for a storage s storing a commodity c in a site v in support timeframe y . The unit of this parameter is MW. The related section for this parameter in the spreadsheet can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “cap-lo-p” represents the parameters \underline{K}_{yvs}^p for corresponding storage tuples. If there is no desired minimum limit for the storage charging/discharging powers, this parameter can be simply set to “0”.

Storage Power Installed, K_{vs}^p , `m.storage_dict['inst-cap-p'][(min(m.stf), sit, sto, com)]`: The parameter K_{vs}^p represents the amount of charging/discharging power of a storage s storing commodity c in a site v and support timeframe y , that is already installed to the energy system at the beginning of the model horizon. The unit of this parameter is MW. The related section for this parameter in the spreadsheet corresponding to the first support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “inst-cap-p” represents the parameters K_{vs}^p for corresponding storage tuples.

Storage Power Upper Bound, \overline{K}_{yvs}^p , `m.storage_dict['cap-up-p'][(stf, sit, sto,`

`com)]`: The parameter \bar{K}_{yvs}^c represents the maximum amount of charging/discharging power allowed of a storage s storing a commodity c in a site v in support timeframe y . The unit of this parameter is MW. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “cap-up-p” represents the parameters \bar{K}_{yvs}^p for corresponding storage tuples. If there is no desired maximum limit for the storage energy content capacities, this parameter can be simply set to “inf”.

Remaining lifetime of installed storages, T_{vs} , `m.storage.loc[(min(m.stf), sit, pro), 'lifetime']`: The parameter T_{vs} represents the remaining lifetime of already installed units. It is used to determine the set $m.inst_sto_tuples$, i.e. to identify for which support timeframes the installed units can still be used.

Storage Energy to Power Ratio, $k_{yvs}^{E/P}$, `m.storage_dict['ep-ratio'][(stf, sit, sto, com)]`: The parameter $k_{yvs}^{E/P}$ represents the linear ratio between the energy and power capacities of a storage s storing a commodity c in a site v in support timeframe y . The unit of this parameter is hours. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Storage” sheet. Here each row represents a storage technology s in a site v that stores a commodity c . The column with the header label “ep-ratio” represents the parameters $k_{yvs}^{E/P}$ for corresponding storage tuples. If there is no desired set ratio for the storage energy and power capacities (which means the storage energy and power capacities can be sized independently from each other), this cell can be left empty.

Storage New Capacity Block, $K_{yvs}^{c,block}$, `m.storage_dict['c-block'][(stf, sit, sto, com)]`: The parameter $K_{yvs}^{c,block}$ represents the capacity of all newly installed units of a storage s at a site v in the support timeframe y . The unit of this parameter is MWh. The related section for this parameter in the spreadsheet can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “c-block” represents the parameters $K_{yvs}^{c,block}$ of the corresponding storage s and site v combinations.

Storage New Power Block, $K_{yvs}^{p,block}$, `m.storage_dict['p-block'][(stf, sit, sto, com)]`: The parameter $K_{yvs}^{p,block}$ represents the power of all newly installed units of a storage s at a site v in the support timeframe y . The unit of this parameter is MW. The related section for this parameter in the spreadsheet can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “c-block” represents the parameters $K_{yvs}^{p,block}$ of the corresponding storage s and site v combinations.

Transmission Technical Parameters

Transmission Efficiency, e_{yaf} , `m.transmission_dict['eff'][(stf, sin, sout, tra, com)]`: The parameter e_{yaf} represents the energy efficiency of a transmission f that transfers a commodity c through an arc a in support timeframe y . Here an arc a defines the connection line from an origin site v_{out} to a destination site v_{in} . The ratio of the output energy amount to input energy amount, gives the energy efficiency of a transmission process. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Transmission” sheet. Here each row represents another combination of transmission f and arc a . The column with the header label “eff” represents the parameters e_{yaf} of the corresponding transmission tuples.

Transmission Capacity Lower Bound, \underline{K}_{yaf} , `m.transmission_dict['cap-lo'][(stf, sin, sout, tra, com)]`: The parameter \underline{K}_{yaf} represents the minimum power output capacity of a transmission f transferring a commodity c through an arc a , that the energy system model is required to have. Here an arc a defines the connection line from an origin site v_{out} to a destination site v_{in} . The unit of this parameter is MW. The related section for this parameter in the spreadsheet corresponding to

the support timeframe can be found under the “Transmission” sheet. Here each row represents another transmission f , arc a combination. The column with the header label “cap-lo” represents the parameters K_{yaf} of the corresponding transmission tuples.

Transmission Capacity Installed, K_{af} , `m.transmission_dict['inst-cap'][(min(m.stf), sin, sout, tra, com)]`: The parameter K_{af} represents the amount of power output capacity of a transmission f transferring a commodity c through an arc a , that is already installed to the energy system at the beginning of the modeling horizon. The unit of this parameter is MW. The related section for this parameter in the spreadsheet corresponding to the first support timeframe can be found under the “Transmission” sheet. Here each row represents another transmission f , arc a combination. The column with the header label “inst-cap” represents the parameters K_{af} of the transmission tuples.

Transmission Capacity Upper Bound, \bar{K}_{yaf} , `m.transmission_dict['cap-up'][(stf, sin, sout, tra, com)]`: The parameter \bar{K}_{yaf} represents the maximum power output capacity of a transmission f transferring a commodity c through an arc a in support timeframe y , that the energy system model is allowed to have. Here an arc a defines the connection line from an origin site v_{out} to a destination site v_{in} . The unit of this parameter is MW. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Transmission” sheet. Here each row represents another transmission f , arc a combination. The column with the header label “cap-up” represents the parameters \bar{K}_{yaf} of the corresponding transmission tuples.

Remaining lifetime of installed transmission, T_{af} , `m.transmission.loc[(min(m.stf), sitin, sitout, tra, com), 'lifetime']`: The parameter T_{af} represents the remaining lifetime of already installed units. It is used to determine the set $m.inst_tra_tuples$, i.e. to identify for which support timeframes the installed units can still be used.

Transmission New Capacity Block, K_{yaf}^{block} , `m.transmission_dict['tra-block'][(stf, sin, sout, tra, com)]`: The parameter K_{yaf}^{block} represents the capacity of all newly installed units of a transmission f transferring a commodity c through an arc a in support timeframe y . The unit of this parameter is MW. The related section for this parameter in the spreadsheet can be found under the “Transmission” sheet. Here each row represents another transmission f , arc a combination. The column with the header label “tra-block” represents the parameters K_{yaf}^{block} of the corresponding transmission tuples.

DCPF Transmission Technical Parameters

Selected transmission lines can be modelled with DC Power Flow and combined with the transport model in an energy system model. The following parameters are only required and included in the model when a transmission line should be modelled with DCPF.

Transmission Reactance, X_{yaf} , `m.transmission_dict['reactance'][(stf, sin, sout, tra, com)]`: The parameter X_{yaf} represents the reactance of a transmission f that transfers a commodity c through an arc a in support timeframe y . Here an arc a defines the connection line from an origin site v_{out} to a destination site v_{in} . Transmission reactance is used to calculate the power flow of DCPF transmission lines. This parameter is required to define a transmission line with the DCPF model and should be given in per unit system. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Transmission” sheet. Here each row represents another combination of transmission f and arc a . The column with the header label “reactance” represents the parameters X_{yaf} of the corresponding transmission tuples. If the parameter is left empty in the spreadsheet, the transmission line will be modelled with transport model as default.

Voltage Angle Difference Limit, \bar{dl}_{yaf} , `m.transmission_dict['difflimit'][(stf, sin, sout, tra, com)]`: The parameter \bar{dl}_{yaf} represents the voltage angle difference limit of

a transmission f that transfers a commodity c through an arc a in support timeframe y . Here an arc a defines the connection line from an origin site v_{out} to a destination site v_{in} . The allowed maximum difference of voltage angles of sites v_{out} and v_{in} is limited with this parameter. This parameter is expected in degrees and a value between 0 and 91 is allowed. This parameter is required to define a transmission line with the DCPF model. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Transmission” sheet. Here each row represents another combination of transmission f and arc a . The column with the header label “difflimit” represents the parameters \overline{dl}_{yaf} of the corresponding transmission tuples.

Transmission Base Voltage, $V_{yafbase}$, `m.transmission_dict['base_voltage'][(stf, sin, sout, tra, com)]`: The parameter $V_{yafbase}$ represents the base voltage of a transmission f that transfers a commodity c through an arc a in support timeframe y . Here an arc a defines the connection line from an origin site v_{out} to a destination site v_{in} . This parameter is used to calculate the power flow of DCPF transmission lines. This parameter is expected in kV and a value greater than 0 is allowed. This parameter is required to define a transmission line with the DCPF model. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “Transmission” sheet. Here each row represents another combination of transmission f and arc a . The column with the header label “base_voltage” represents the parameters $V_{yafbase}$ of the corresponding transmission tuples.

Demand Side Management Technical Parameters

DSM Efficiency, e_{yvc} , `m.dsm_dict['eff'][(stf, sit, com)]`: The parameter e_{yvc} represents the efficiency of the DSM process, i.e., the fraction of DSM upshift that is benefiting the system via the corresponding DSM downshifts of demand commodity c in site v and support timeframe y . The parameter is given as a fraction with “1” meaning a perfect recovery of the DSM upshift. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “DSM” sheet. Here each row represents another DSM potential for demand commodity c in site v . The column with the header label “eff” represents the parameters e_{yvc} of the corresponding DSM tuples.

DSM Delay Time, y_{yvc} , `m.dsm_dict['delay'][(stf, sit, com)]`: The delay time y_{yvc} restricts how long the time difference between an upshift and its corresponding downshifts may be for demand commodity c in site v and support timeframe y . The parameter is given in h. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “DSM” sheet. Here each row represents another DSM potential for demand commodity c in site v . The column with the header label “delay” represents the parameters y_{yvc} of the corresponding DSM tuples.

DSM Recovery Time, o_{yvc} , `m.dsm_dict['recov'][(stf, sit, com)]`: The recovery time o_{yvc} prevents the DSM system to continuously shift demand. During the recovery time, all upshifts of demand commodity c in site v and support timeframe y may not exceed the product of the delay time and the maximal upshift capacity. The parameter is given in h. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “DSM” sheet. Here each row represents another DSM potential for demand commodity c in site v . The column with the header label “recov” represents the parameters o_{yvc} of the corresponding DSM tuples. If no limitation via this parameter is desired it has to be set to values lower than the delay time y_{yvc} .

DSM Maximal Upshift Per Hour, \overline{K}_{yvc}^{up} , MW, `m.dsm_dict['cap-max-up'][(stf, sit, com)]`: The DSM upshift capacity \overline{K}_{yvc}^{up} limits the total upshift per hour for a DSM potential of demand commodity c in site v and support timeframe y . The parameter is given in MW. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “DSM” sheet. Here each row represents another DSM potential for demand commodity c in site v . The column with the header label “cap-max-up” represents the parameters \overline{K}_{yvc}^{up} of the corresponding DSM tuples.

DSM Maximal Downshift Per Hour, $\bar{K}_{yvc}^{\text{down}}$, MW, `m.dsm_dict['cap-max-do'][(stf, sit, com)]`: The DSM downshift capacity $\bar{K}_{yvc}^{\text{down}}$ limits the total downshift per hour for a DSM potential of demand commodity c in site v and support timeframe y . The parameter is given in MW. The related section for this parameter in the spreadsheet corresponding to the support timeframe can be found under the “DSM” sheet. Here each row represents another DSM potential for demand commodity c in site v . The column with the header label “cap-max-do” represents the parameters $\bar{K}_{yvc}^{\text{down}}$ of the corresponding DSM tuples.

Economic Parameters

Table 6: Table: Economic Model Parameters

Parameter	Unit	Description
j	–	Global Discount rate
D_y	–	Factor for any payment made in modeled year y
I_y	–	Factor for any investment made in modeled year y
\bar{L}_{cost}	€	Maximum total system costs (if CO2 is minimized)
Commodity Economic Parameters		
k_{yvc}^{fuel}	€/MWh	Stock Commodity Fuel Costs
k_{yvc}^{env}	€/MWh	Environmental Commodity Costs
k_{yvc}^{bs}	€/MWh	Buy/Sell Commodity Buy/Sell Costs
k_{yvc}^{bs}	–	Multiplier for Buy/Sell Commodity Buy/Sell Costs
Process Economic Parameters		
i_{yvp}	–	Weighted Average Cost of Capital for Process
z_{yvp}	–	Process Depreciation Period
k_{yvp}^{inv}	€/MW	Process Capacity Investment Costs
k_{yvp}^{fix}	€/(MW a)	Annual Process Capacity Fixed Costs
k_{yvp}^{var}	€/MWh	Process Throughput Variable Costs
P_{yvp}^{start}	€/MW	Process Start-up Cost
Storage Economic Parameters		
i_{yvs}	–	Weighted Average Cost of Capital for Storage
z_{yvs}	–	Storage Depreciation Period
$k_{yvs}^{\text{p,inv}}$	€/MW	Storage Power Investment Costs
$k_{yvs}^{\text{p,fix}}$	€/(MW a)	Annual Storage Power Fixed Costs
$k_{yvs}^{\text{p,var}}$	€/MWh	Storage Power Variable Costs
$k_{yvs}^{\text{c,inv}}$	€/MWh	Storage Size Investment Costs
$k_{yvs}^{\text{c,fix}}$	€/(MWh a)	Annual Storage Size Fixed Costs
$k_{yvs}^{\text{c,var}}$	€/MWh	Storage Usage Variable Costs
Transmission Economic Parameters		
i_{yvf}	–	Weighted Average Cost of Capital for Transmission
z_{yaf}	–	Transmission Depreciation Period
k_{yaf}^{inv}	€/MW	Transmission Capacity Investment Costs
k_{yaf}^{fix}	€/(MW a)	Annual Transmission Capacity Fixed Costs
k_{yaf}^{var}	€/MWh	Transmission Usage Variable Costs

Discount rate, j , `m.global_prop.xls('Discount rate', level=1).loc[m.global_prop.index.min()[0]]['value']`: The discount rate j is used to calculate the present value of future costs. It is set in the worksheet “Global” in the input file of the first support

timeframe.

Factor for future payments, D_y : The parameter D_y is a multiplier that has to be factored into all cost terms apart from the invest costs in intertemporal planning based on support timeframes. All other cost terms for the support timeframe y are multiplied directly with this factor to find the present value of the sum of costs in support timeframe y and all non-modeled time frames until the next modeled time frame y_{+1} , which are identical to the support timeframe with the modeling approach taken:

$$D_y = (1 + j)^{1-(y-y_{\min})} \cdot \frac{1 - (1 + j)^{-(y_{+1}-y+1)}}{j}$$

In script `modelhelper.py` the factor D_y is implemented as the product of the functions:

```
def discount_factor(stf, m):
    """Discount for any payment made in the year stf
    """
    discount = (m.global_prop.xls('Discount rate', level=1)
                .loc[m.global_prop.index.min()[0]]['value'])

    return (1 + discount) ** (1 - (stf - m.global_prop.index.min()[0]))
```

and

```
def effective_distance(dist, m):
    """Factor for variable, fuel, purchase, sell, and fix costs.
    Calculated by repetition of modeled stfs and discount utility.
    """
    discount = (m.global_prop.xls('Discount rate', level=1)
                .loc[m.global_prop.index.min()[0]]['value'])

    if discount == 0:
        return dist
    else:
        return (1 - (1 + discount) ** (-dist)) / discount
```

Factor for investment made in support timeframe y , I_y : The parameter I_y is a multiplier that has to be factored into the invest costs in intertemporal planning based on support timeframes. The book value of the total invest costs per capacity in support timeframe y is multiplied with this factor to find the present value of the sum of costs of all annual payments made for this investment within the modeling horizon. The calculation of this parameter requires several case distinctions and is given by:

- $i \neq 0, j \neq 0$:

$$I_y = (1 + j)^{1-(y-y_{\min})} \cdot \frac{i}{j} \cdot \left(\frac{1+i}{1+j} \right)^n \cdot \frac{(1+j)^n - (1+j)^{n-k}}{(1+i)^n - 1}$$

- $i = 0, j = 0$:

$$I_y = \frac{k}{n}$$

- $i \neq 0, j = 0$:

$$I_y = k \cdot \frac{(1+i)^n \cdot i}{(1+i)^n - 1}$$

- $i = 0, j \neq 0$:

$$I_y = \frac{1}{n} \cdot (1+j)^{-m} \cdot \frac{(1+j)^k - 1}{(1+j)^k \cdot j}$$

where k is the number of annualized payments that have to be made within the modeling horizon, n the depreciation period and i the weighted average cost of capital. Note that the parameters i and n take different values for different unit tuples.

In script `modelhelper.py` the factor I_y is implemented with the function:

```
def invcost_factor(dep_prd, interest, discount=None, year_built=None,
                  stf_min=None):
    """Investment cost factor formula.
    Evaluates the factor multiplied to the invest costs
    for depreciation duration and interest rate.
    Args:
        dep_prd: depreciation period (years)
        interest: interest rate (e.g. 0.06 means 6 %)
        year_built: year utility is built
        discount: discount rate for intertemporal planning
    """
    # invcost factor for non intertemporal planning
    if discount is None:
        if interest == 0:
            return 1 / dep_prd
        else:
            return ((1 + interest) ** dep_prd * interest /
                    ((1 + interest) ** dep_prd - 1))
    # invcost factor for intertemporal planning
    elif discount == 0:
        if interest == 0:
            return 1
        else:
            return (dep_prd * ((1 + interest) ** dep_prd * interest) /
                    ((1 + interest) ** dep_prd - 1))
    else:
        if interest == 0:
            return ((1 + discount) ** (1 - (year_built-stf_min))) *
                    ((1 + discount) ** dep_prd - 1) /
                    (dep_prd * discount * (1 + discount) ** dep_prd))
        else:
            return ((1 + discount) ** (1 - (year_built-stf_min))) *
                    (interest * (1 + interest) ** dep_prd *
                     ((1 + discount) ** dep_prd - 1)) /
                    (discount * (1 + discount) ** dep_prd *
                     ((1+interest) ** dep_prd - 1)))
```

In this formulation also payments after the modeled time horizon are being made. To fix this the overpay is subtracted via:

```
def overpay_factor(dep_prd, interest, discount, year_built, stf_min, stf_
    ↪end):
    """Overpay value factor formula.
    Evaluates the factor multiplied to the invest costs
    for all annuity payments of a unit after the end of the
    optimization period.
    Args:
        dep_prd: depreciation period (years)
        interest: interest rate (e.g. 0.06 means 6 %)
        year_built: year utility is built
        discount: discount rate for intertemporal planning
```

(continues on next page)

(continued from previous page)

```

    k: operational time after simulation horizon
    """

    op_time = (year_built + dep_prd) - stf_end - 1

    if discount == 0:
        if interest == 0:
            return op_time / dep_prd
        else:
            return (op_time * ((1 + interest) ** dep_prd * interest) /
                    ((1 + interest) ** dep_prd - 1))
    else:
        if interest == 0:
            return ((1 + discount) ** (1 - (year_built - stf_min))) *
                    ((1 + discount) ** op_time - 1) /
                    (dep_prd * discount * (1 + discount) ** dep_prd)
        else:
            return ((1 + discount) ** (1 - (year_built - stf_min))) *
                    (interest * (1 + interest) ** dep_prd *
                     ((1 + discount) ** op_time - 1)) /
                    (discount * (1 + discount) ** dep_prd *
                     ((1 + interest) ** dep_prd - 1))

```

In case of negative values this overpay factor is set to zero afterwards.

Maximum total system cost, \bar{L}_{cost} , `m.global_prop.loc[(min(m.stf), 'Cost budget'), 'value']`: This parameter restricts the total present costs over the entire modeling horizon. It is only sensible and active when the objective is a minimization of CO2 emissions.

Commodity Economic Parameters

Stock Commodity Fuel Costs, k_{vc}^{fuel} , `m.commodity_dict['price'][c]`: The parameter k_{yvc}^{fuel} represents the book cost for purchasing one unit (1 MWh) of a stock commodity c ($\forall c \in C_{\text{stock}}$) in modeled timeframe y in a site v ($\forall v \in V$). The unit of this parameter is €/MWh. The related section for this parameter in the spreadsheet belonging the support timeframe y can be found in the “Commodity” sheet. Here each row represents another commodity tuple c_{yvc} and the column of stock commodity tuples ($\forall q = \text{“Stock”}$) in this sheet with the header label “price” represents the corresponding parameter k_{yvc}^{fuel} .

Environmental Commodity Costs, k_{yvc}^{env} , `m.commodity_dict['price'][c]`: The parameter k_{yvc}^{env} represents the book cost for producing/emitting one unit (1 t, 1 kg, ...) of an environmental commodity c ($\forall c \in C_{\text{env}}$) in support timeframe y in a site v ($\forall v \in V$). The unit of this parameter is €/t (i.e. per unit of output). The related section for this parameter in the spreadsheet corresponding to support timeframe y is the “Commodity” sheet. Here, each row represents a commodity tuple c_{yvc} and the fourth column of environmental commodity tuples ($\forall q = \text{“Env”}$) in this sheet with the header label “price” represents the corresponding parameter k_{yvc}^{env} .

Buy/Sell Commodity Buy/Sell Costs, k_{yvct}^{bs} , `m.buy_sell_price_dict[c[2], [(c[0], t_m)]]`: The parameter k_{yvct}^{bs} represents the purchase/buy cost for purchasing/selling one unit (1 MWh) of a buy/sell commodity c ($\forall c \in C_{\text{buy}}$)($\forall c \in C_{\text{sell}}$) in support timeframe y in a site v ($\forall v \in V$) at timestep t ($\forall t \in T_m$). The unit of this parameter is €/MWh. The related section for this parameter in the spreadsheet can be found in the “Buy-Sell-Price” sheet. Here each column represents a commodity tuple and the row values provide the timestep information.

Multiplier for Buy/Sell Commodity Buy/Sell Costs, k_{yvc}^{bs} , `m.commodity_dict['price'][c]`: The parameter k_{yvc}^{bs} is a multiplier for the buy/sell time series. It represents the factor on the purchase/buy cost for purchasing/selling one unit (1 MWh) of a buy/sell commodity c ($\forall c \in C_{\text{buy}}/(\forall c \in C_{\text{sell}})$) in support timeframe y in a site v ($\forall v \in V$). This parameter is unitless. The related section for this parameter in the spreadsheet belonging to support timeframe y can be found in the “Commodity” sheet. Here each row represents another commodity tuple c_{yvc} and the column of Buy/Sell commodity tuples ($\forall q = \text{“Buy/Sell”}$) in this sheet with the header label “price” represents the corresponding parameter k_{yvc}^{bs} .

Process Economic Parameters

Weighted Average Cost of Capital for Process, i_{yvp} , : The parameter i_{yvp} represents the weighted average cost of capital for a process technology p in support timeframe y in a site v . The weighted average cost of capital gives the interest rate (%) of costs for capital after taxes. The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Process” sheet. Here each row represents another process tuple and the column with the header label “wacc” represents the parameters i_{yvp} . The parameter is given as a percentage, where “0.07” means 7%.

Process Depreciation Period, z_{yvp} : The parameter z_{yvp} represents the depreciation period of a process p built in support timeframe y in a site v . The depreciation period gives the economic and technical lifetime of a process investment. It thus features in the calculation of the invest cost factor and determines the end of operation of the process. The unit of this parameter is “a”, where “a” represents a year of 8760 hours. The related section for this parameter in the spreadsheet can be found under the “Process” sheet. Here each row represents another process tuple and the column with the header label “depreciation” represents the parameters z_{yvp} .

Process Capacity Investment Costs, k_{yvp}^{inv} , `m.process_dict['inv-cost'][p]`: The parameter k_{yvp}^{inv} represents the book value of the investment cost for adding one unit new capacity of a process technology p in support timeframe y in a site v . The unit of this parameter is €/MW. To get the full impact of the investment within the modeling horizon this parameter is multiplied with the factor for the investment made in modeled year y I_y . The process capacity investment cost is to be given as an input by the user. The related section for the process capacity investment cost in the spreadsheet representing the support timeframe y can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “inv-cost” represents the process capacity investment costs of the corresponding process p and site v combinations.

Process Capacity Fixed Costs, k_{yvp}^{fix} , `m.process_dict['fix-cost'][p]`: The parameter k_{yvp}^{fix} represents the fix cost per one unit capacity κ_{yvp} of a process technology p in support timeframe y in a site v , that is charged annually. The unit of this parameter is €/(MW a). The related section for this parameter in the spreadsheet corresponding to the support timeframe y can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “fix-cost” represents the parameters k_{yvp}^{fix} of the corresponding process p and site v combinations.

Process Variable Costs, k_{yvp}^{var} , `m.process_dict['var-cost'][p]`: The parameter k_{yvp}^{var} represents the book value of the variable cost per one unit energy throughput τ_{yvpt} through a process technology p in a site v in support timeframe y . The unit of this parameter is €/MWh. The related section for this parameter in the spreadsheet corresponding to the support timeframe y can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “var-cost” represents the parameters k_{yvp}^{var} of the corresponding process p and site v combinations.

Process Start-up Cost, P_{yvp}^{start} , `m.process_dict['start-cost'][(stf, sit, pro)]`: The parameter P_{yvp}^{start} represents the cost inquired by the starting of a process p at a site v in the support timeframe y . The unit of this parameter is the currency used in the support timeframe y . The related

section for this parameter in the spreadsheet can be found under the “Process” sheet. Here each row represents another process p in a site v and the column with the header label “start-cost” represents the parameters P_{yvp}^{start} of the corresponding process p and site v combinations.

Storage Economic Parameters

Weighted Average Cost of Capital for Storage, i_{yvs} : The parameter i_{yvs} represents the weighted average cost of capital for a storage technology s in a site v and support timeframe y . The weighted average cost of capital gives the interest rate(%) of costs for capital after taxes. The related section for this parameter in the spreadsheet corresponding to the support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “wacc” represents the parameters i_{yvs} of the corresponding storage s and site v combinations. The parameter is given as a percentage, where “0.07” means 7%.

Storage Depreciation Period, z_{yvs} , (a): The parameter z_{yvs} represents the depreciation period of a storage s in a site v built in support timeframe y . The depreciation period gives the economic and technical lifetime of a storage investment. It thus features in the calculation of the invest cost factor and determines the end of operation of the storage. The unit of this parameter is “a”, where “a” represents a year of 8760 hours. The related section for this parameter in the spreadsheet corresponding to the support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “depreciation” represents the parameters z_{yvs} of the corresponding storage s and site v combinations.

Storage Power Investment Costs, $k_{yvs}^{\text{p,inv}}$, $\text{m.storage_dict}['\text{inv-cost-p}'][s]$: The parameter $k_{yvs}^{\text{p,inv}}$ represents the book value of the total investment cost for adding one unit new power output capacity of a storage technology s in a site v in support timeframe y . The unit of this parameter is €/MW. To get the full impact of the investment within the modeling horizon this parameter is multiplied with the factor for the investment made in modeled year y I_y . The related section for the storage power output capacity investment cost in the spreadsheet corresponding to the support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “inv-cost-p” represents the storage power output capacity investment cost of the corresponding storage s and site v combinations.

Annual Storage Power Fixed Costs, $k_{yvs}^{\text{p,fix}}$, $\text{m.storage_dict}['\text{fix-cost-p}'][s]$: The parameter $k_{yvs}^{\text{p,fix}}$ represents the fix cost per one unit power output capacity of a storage technology s in a site v and support timeframe y , that is charged annually. The unit of this parameter is €/(MW a). The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “fix-cost-p” represents the parameters $k_{yvs}^{\text{p,fix}}$ of the corresponding storage s and site v combinations.

Storage Power Variable Costs, $k_{yvs}^{\text{p,var}}$, $\text{m.storage_dict}['\text{var-cost-p}'][s]$: The parameter $k_{yvs}^{\text{p,var}}$ represents the variable cost per unit energy, that is stored in or retrieved from a storage technology s in a site v in support timeframe y . The unit of this parameter is €/MWh. The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “var-cost-p” represents the parameters $k_{yvs}^{\text{p,var}}$ of the corresponding storage s and site v combinations.

Storage Size Investment Costs, $k_{yvs}^{\text{c,inv}}$, $\text{m.storage_dict}['\text{inv-cost-c}'][s]$: The parameter $k_{yvs}^{\text{c,inv}}$ represents the book value of the total investment cost for adding one unit new storage capacity to a storage technology s in a site v in support timeframe y . The unit of this parameter is €/MWh. To get the full impact of the investment within the modeling horizon this parameter is multiplied with

the factor for the investment made in modeled year y I_y . The related section for the storage content capacity investment cost in the spreadsheet corresponding to support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “inv-cost-c” represents the storage content capacity investment cost of the corresponding storage s and site v combinations.

Annual Storage Size Fixed Costs, $k_{yvs}^{c,fix}$, `m.storage_dict['fix-cost-c'][s]`: The parameter $k_{yvs}^{c,fix}$ represents the fix cost per year per one unit storage content capacity of a storage technology s in a site v in support timeframe y . The unit of this parameter is €/MWh a). The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “fix-cost-c” represents the parameters $k_{yvs}^{c,fix}$ of the corresponding storage s and site v combinations.

Storage Usage Variable Costs, $k_{yvs}^{c,var}$, `m.storage_dict['var-cost-c'][s]`: The parameter $k_{yvs}^{c,var}$ represents the variable cost per unit energy, that is conserved in a storage technology s in a site v in support timeframe y . The unit of this parameter is €/MWh. The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Storage” sheet. Here each row represents another storage s in a site v and the column with the header label “var-cost-c” represents the parameters $k_{yvs}^{c,var}$ of the corresponding storage s and site v combinations. The value of this parameter is usually set to zero, but the parameter can be taken advantage of if the storage has a short term usage or has an increased devaluation due to usage, compared to amount of energy stored.

Transmission Economic Parameters

Weighted Average Cost of Capital for Transmission, i_{yvf} , : The parameter i_{yvf} represents the weighted average cost of capital for a transmission f transferring commodities through an arc a built in support timeframe y . The weighted average cost of capital gives the interest rate(%) of costs for capital after taxes. The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Transmission” sheet. Here each row represents another transmission f transferring commodities through an arc a and the column with the header label “wacc” represents the parameters i_{yvf} of the corresponding transmission f and arc a combinations. The parameter is given as a percentage, where “0.07” means 7%.

Transmission Depreciation Period, z_{yaf} , (a): The parameter z_{yaf} represents the depreciation period of a transmission f transferring commodities through an arc a built in support timeframe y . The depreciation period of gives the economic and technical lifetime of a transmission investment. It thus features in the calculation of the invest cost factor and determines the end of operation of the transmission. The unit of this parameter is “a”, where “a” represents a year of 8760 hours. The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Transmission” sheet. Here each row represents another transmission f transferring commodities through an arc a and the column with the header label “depreciation” represents the parameters z_{yaf} of the corresponding transmission f and arc a combinations.

Transmission Capacity Investment Costs, k_{yaf}^{inv} , `m.transmission_dict['inv-cost'][t]`: The parameter k_{yaf}^{inv} represents the book value of the investment cost for adding one unit new transmission capacity to a transmission f transferring commodities through an arc a in support timeframe y . To get the full impact of the investment within the modeling horizon this parameter is multiplied with the factor for the investment made in modeled year y I_y . The unit of this parameter is €/MW. The related section for the transmission capacity investment cost in the spreadsheet corresponding to support timeframe y can be found under the “Transmission” sheet. Here each row represents another transmission f transferring commodities through an arc a and the column with the header label “inv-cost” represents the transmission capacity investment cost of the corresponding transmission f and arc a combinations.

Annual Transmission Capacity Fixed Costs, k_{yaf}^{fix} , $m.\text{transmission_dict}['\text{fix-cost}'][t]$: The parameter k_{yaf}^{fix} represents the annual fix cost per one unit capacity of a transmission f transferring commodities through an arc a . The unit of this parameter is €/ (MW a). The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Transmission” sheet. Here each row represents another transmission f transferring commodities through an arc a and the column with the header label “fix-cost” represents the parameters k_{yaf}^{fix} of the corresponding transmission f and arc a combinations.

Transmission Usage Variable Costs, k_{yaf}^{var} , $m.\text{transmission_dict}['\text{var-cost}'][t]$: The parameter k_{yaf}^{var} represents the variable cost per unit energy, that is transferred with a transmission f through an arc a . The unit of this parameter is €/ MWh. The related section for this parameter in the spreadsheet corresponding to support timeframe y can be found under the “Transmission” sheet. Here each row represents another transmission f transferring commodities through an arc a and the column with the header label “var-cost” represents the parameters k_{yaf}^{var} of the corresponding transmission f and arc a combinations.

Equations

Objective function

There are two possible choices of objective function for urbs problems, either the costs (default option) or the total CO2-emissions can be minimized.

If the total CO2-emissions are minimized the objective function takes the form:

$$w \sum_{t \in T_m} \sum_{v \in V} -\text{CB}(v, \text{CO}_2, t)$$

In script `model.py` the global CO2 emissions are defined and calculated by the following code fragment:

```
def co2_rule(m):
    co2_output_sum = 0
    for stf in m.stf:
        for tm in m.tm:
            for sit in m.sit:
                # minus because negative commodity_balance represents
                # creation of that commodity.
                if m.mode['int']:
                    co2_output_sum += (- commodity_balance(m, tm, stf, sit,
→ 'CO2') *
                                                    m.typeperiod['weight_typeperiod
→'][(stf, tm)] *
                                                    m.weight * stf_dist(stf, m))
                else:
                    co2_output_sum += (- commodity_balance(m, tm, stf, sit,
→ 'CO2') *
                                                    m.weight)

    return (co2_output_sum)
```

In the default case the total system costs are minimized. These variable total system costs ζ are calculated by the cost function. The cost function is the objective function of the optimization model. Minimizing the value of the variable total system cost would give the most reasonable solution for the modelled

energy system. The formula of the cost function expressed in mathematical notation is as following:

)The calculation of the variable total system cost is given in `model.py` by the following code fragment.

```
def cost_rule(m):
    return pyomo.summation(m.costs)
```

The variable total system cost ζ is basically calculated by the summation of every type of total costs. As previously mentioned in section *Cost Types*, these cost types are : Investment, Fix, Variable, Fuel, Revenue, Purchase, Start-up and Environmental.

In script `model.py` the individual cost functions are calculated by the following code fragment:

```
def def_costs_rule(m, cost_type):
    #Calculate total costs by cost type.
    #Sums up process activity and capacity expansions
    #and sums them in the cost types that are specified in the set
    #m.cost_type. To change or add cost types, add/change entries
    #there and modify the if/elif cases in this function accordingly.
    #Cost types are
    # - Investment costs for process power, storage power and
    #   storage capacity. They are multiplied by the investment
    #   factors. Rest values of units are subtracted.
    # - Fixed costs for process power, storage power and storage
    #   capacity.
    # - Variables costs for usage of processes, storage and transmission.
    # - Fuel costs for stock commodity purchase.

    if cost_type == 'Invest':
        cost = \
            sum(m.cap_pro_new[p] *
                m.process_dict['inv-cost'][p] *
                m.process_dict['invcost-factor'][p]
                for p in m.pro_tuples)
        if m.mode['int']:
            cost -= \
                sum(m.cap_pro_new[p] *
                    m.process_dict['inv-cost'][p] *
                    m.process_dict['overpay-factor'][p]
                    for p in m.pro_tuples)
        if m.mode['tra']:
            # transmission_cost is defined in transmission.py
            cost += transmission_cost(m, cost_type)
        if m.mode['sto']:
            # storage_cost is defined in storage.py
            cost += storage_cost(m, cost_type)
        return m.costs[cost_type] == cost

    elif cost_type == 'Fixed':
        cost = \
            sum(m.cap_pro[p] * m.process_dict['fix-cost'][p] *
                m.process_dict['cost_factor'][p]
                for p in m.pro_tuples)
        if m.mode['tra']:
            cost += transmission_cost(m, cost_type)
```

(continues on next page)

(continued from previous page)

```

    if m.mode['sto']:
        cost += storage_cost(m, cost_type)
        return m.costs[cost_type] == cost

    elif cost_type == 'Variable':
        cost = \
            sum(m.tau_pro[(tm,) + p] * m.weight * m.typeperiod['weight_
→typeperiod'][(m.stf_list[0],tm)] *
                m.process_dict['var-cost'][p] *
                m.process_dict['cost_factor'][p]
                for tm in m.tm
                for p in m.pro_tuples)
        if m.mode['tra']:
            cost += transmission_cost(m, cost_type)
        if m.mode['sto']:
            cost += storage_cost(m, cost_type)
        return m.costs[cost_type] == cost

    elif cost_type == 'Fuel':
        return m.costs[cost_type] == sum(
            m.e_co_stock[(tm,) + c] * m.weight * m.typeperiod['weight_
→typeperiod'][(m.stf_list[0],tm)] *
            m.commodity_dict['price'][c] *
            m.commodity_dict['cost_factor'][c]
            for tm in m.tm for c in m.com_tuples
            if c[2] in m.com_stock)

    elif cost_type == 'Start-up':
        if m.mode['onoff']:
            cost = sum(m.start_up[(tm,) + p] * m.weight *
                m.start_price_dict[p] * m.cap_pro[p] *
                m.process_dict['cost_factor'][p]
                for tm in m.tm
                for p in m.pro_start_up_tuples)
            return m.costs[cost_type] == cost
        else:
            return m.costs[cost_type] == 0

    elif cost_type == 'Environmental':
        return m.costs[cost_type] == sum(
            - commodity_balance(m, tm, stf, sit, com) * m.weight * m.
→typeperiod['weight_typeperiod'][(m.stf_list[0],tm)] *
            m.commodity_dict['price'][(stf, sit, com, com_type)] *
            m.commodity_dict['cost_factor'][(stf, sit, com, com_type)]
            for tm in m.tm
            for stf, sit, com, com_type in m.com_tuples
            if com in m.com_env)

    # Revenue and Purchase costs defined in BuySellPrice.py
    elif cost_type == 'Revenue':
        return m.costs[cost_type] == revenue_costs(m)

    elif cost_type == 'Purchase':
        return m.costs[cost_type] == purchase_costs(m)

```

(continues on next page)

(continued from previous page)

```

else:
    raise NotImplementedError("Unknown cost type.")

```

Constraints

Commodity Constraints

Commodity Balance The function commodity balance calculates the in- and outflows into all processes, storages and transmission of a commodity c in a site v in support timeframe y at a timestep t . The value of the function CB being greater than zero $CB > 0$ means that the presence of the commodity c in the site v in support timeframe y at the timestep t is getting by the interaction with the technologies given above. Correspondingly, the value of the function being less than zero means that the presence of the commodity in the site at the timestep is getting more than before by the technologies given above. The mathematical explanation of this rule for general problems is explained in [Energy Storage](#).

In script `modelhelper.py` the value of the commodity balance function $CB(y, v, c, t)$ is calculated by the following code fragment:

```

def commodity_balance(m, tm, stf, sit, com):
    """Calculate commodity balance at given timestep.
    For a given commodity co and timestep tm, calculate the balance of
    consumed (to process/storage/transmission, counts positive) and
    →provided
    (from process/storage/transmission, counts negative) commodity flow.
    →Used
    as helper function in create_model for constraints on demand and stock
    commodities.
    Args:
        m: the model object
        tm: the timestep
        site: the site
        com: the commodity
    Returns
        balance: net value of consumed (positive) or provided (negative)
    →power
    """
    balance = (sum(m.e_pro_in[(tm, stframe, site, process, com)]
        # usage as input for process increases balance
        for stframe, site, process in m.pro_tuples
        if site == sit and stframe == stf and
        (stframe, process, com) in m.r_in_dict) -
        sum(m.e_pro_out[(tm, stframe, site, process, com)]
        # output from processes decreases balance
        for stframe, site, process in m.pro_tuples
        if site == sit and stframe == stf and
        (stframe, process, com) in m.r_out_dict))
    if m.mode['tra']:
        balance += transmission_balance(m, tm, stf, sit, com)
    if m.mode['sto']:
        balance += storage_balance(m, tm, stf, sit, com)

    return balance

```


where the two functions introducing the partly balances for transmissions and storages, respectively, are given by:

```
def transmission_balance(m, tm, stf, sit, com):
    """called in commodity balance
    For a given commodity co and timestep tm, calculate the balance of
    import and export """

    return (sum(m.e_tra_in[(tm, stframe, site_in, site_out,
                           transmission, com)]
               # exports increase balance
               for stframe, site_in, site_out, transmission, commodity
               in m.tra_tuples
               if (site_in == sit and stframe == stf and
                   commodity == com)) -
            sum(m.e_tra_out[(tm, stframe, site_in, site_out,
                           transmission, com)]
               # imports decrease balance
               for stframe, site_in, site_out, transmission, commodity
               in m.tra_tuples
               if (site_out == sit and stframe == stf and
                   commodity == com)))
```

```
def storage_balance(m, tm, stf, sit, com):
    """called in commodity balance
    For a given commodity co and timestep tm, calculate the balance of
    storage input and output """

    return sum(m.e_sto_in[(tm, stframe, site, storage, com)] -
               m.e_sto_out[(tm, stframe, site, storage, com)]
               # usage as input for storage increases consumption
               # output from storage decreases consumption
               for stframe, site, storage, commodity in m.sto_tuples
               if site == sit and stframe == stf and commodity == com)
```

Vertex Rule: The vertex rule is the main constraint that has to be satisfied for every commodity. It represents a version of “Kirchhoff’s current law” or local energy conservation. This constraint is defined differently for each commodity type. The inequality requires, that any imbalance ($CB > 0$, $CB < 0$) of a commodity c in a site v and support timeframe y at a timestep t to be balanced by a corresponding source term or demand. The rule is not defined for environmental or SupIm commodities. The mathematical explanation of this rule is given in *Minimal optimization model*.

In script `model.py` the constraint vertex rule is defined and calculated by the following code fragments:

```
m.res_vertex = pyomo.Constraint(
    m.tm, m.com_tuples,
    rule=res_vertex_rule,
    doc='storage + transmission + process + source + buy - sell == demand')
```

```
def res_vertex_rule(m, tm, stf, sit, com, com_type):
    # environmental or supim commodities don't have this constraint (yet)
    if com in m.com_env:
        return pyomo.Constraint.Skip
    if com in m.com_supim:
        return pyomo.Constraint.Skip
```

(continues on next page)

(continued from previous page)

```

# helper function commodity_balance calculates balance from input to
# and output from processes, storage and transmission.
# if power_surplus > 0: production/storage/imports create net positive
#                        amount of commodity com
# if power_surplus < 0: production/storage/exports consume a net
#                        amount of the commodity com
power_surplus = - commodity_balance(m, tm, stf, sit, com)

# if com is a stock commodity, the commodity source term e_co_stock
# can supply a possibly negative power_surplus
if com in m.com_stock:
    power_surplus += m.e_co_stock[tm, stf, sit, com, com_type]

# if Buy and sell prices are enabled
if m.mode['bsp']:
    power_surplus += bsp_surplus(m, tm, stf, sit, com, com_type)

# if com is a demand commodity, the power_surplus is reduced by the
# demand value; no scaling by m.dt or m.weight is needed here, as this
# constraint is about power (MW), not energy (MWh)
if com in m.com_demand:
    try:
        power_surplus -= m.demand_dict[(sit, com)][(stf, tm)]
    except KeyError:
        pass

if m.mode['dsm']:
    power_surplus += dsm_surplus(m, tm, stf, sit, com)

return power_surplus == 0

```

where the two functions introducing the effects of Buy/Sell or DSM events, respectively, are given by:

```

def bsp_surplus(m, tm, stf, sit, com, com_type):

    power_surplus = 0

    # if com is a sell commodity, the commodity source term e_co_sell
    # can supply a possibly positive power_surplus
    if com in m.com_sell:
        power_surplus -= m.e_co_sell[tm, stf, sit, com, com_type]

    # if com is a buy commodity, the commodity source term e_co_buy
    # can supply a possibly negative power_surplus
    if com in m.com_buy:
        power_surplus += m.e_co_buy[tm, stf, sit, com, com_type]

    return power_surplus

```

```

def dsm_surplus(m, tm, stf, sit, com):
    """ called in vertex rule
        calculate dsm surplus"""
    if (stf, sit, com) in m.dsm_site_tuples:
        return (- m.dsm_up[tm, stf, sit, com] +
                sum(m.dsm_down[t, tm, stf, sit, com]

```

(continues on next page)

(continued from previous page)

```

        for t in dsm_time_tuples(
            tm, m.timesteps[1:],
            max(int(1 / m.dt *
                m.dsm_dict['delay'][(stf, sit, com)]), 1))))
    else:
        return 0

```

Stock Per Step Rule: The constraint stock per step rule applies only for commodities of type “Stock” ($c \in C_{st}$). This constraint limits the amount of stock commodity $c \in C_{st}$, that can be used by the energy system in the site v in support timeframe y at the timestep t . This amount is limited by the product of the parameter maximum stock supply limit per hour \bar{l}_{yvc} and the timestep length Δt . The mathematical explanation of this rule is given in *Minimal optimization model*.

In script `model.py` the constraint stock per step rule is defined and calculated by the following code fragment:

```

m.res_stock_step = pyomo.Constraint(
    m.tm, m.com_tuples,
    rule=res_stock_step_rule,
    doc='stock commodity input per step <= commodity.maxperstep')

```

```

def res_stock_step_rule(m, tm, stf, sit, com, com_type):
    if com not in m.com_stock:
        return pyomo.Constraint.Skip
    else:
        return (m.e_co_stock[tm, stf, sit, com, com_type] <=
            m.dt * m.commodity_dict['maxperhour']
                [(stf, sit, com, com_type)])

```

Total Stock Rule: The constraint total stock rule applies only for commodities of type “Stock” ($c \in C_{st}$). This constraint limits the amount of stock commodity $c \in C_{st}$, that can be used annually by the energy system in the site v and support timeframe y . This amount is limited by the parameter maximum annual stock supply limit per vertex \bar{L}_{yvc} . The annual usage of stock commodity is calculated by the sum of the products of the parameter weight w and the parameter stock commodity source term ρ_{yvct} , summed over all timesteps $t \in T_m$. The mathematical explanation of this rule is given in *Minimal optimization model*.

In script `model.py` the constraint total stock rule is defined and calculated by the following code fragment:

```

m.res_stock_total = pyomo.Constraint(
    m.com_tuples,
    rule=res_stock_total_rule,
    doc='total stock commodity input <= commodity.max')

```

```

def res_stock_total_rule(m, stf, sit, com, com_type):
    if com not in m.com_stock:
        return pyomo.Constraint.Skip
    else:
        # calculate total consumption of commodity com
        total_consumption = 0
        for tm in m.tm:
            total_consumption += (
                m.e_co_stock[tm, stf, sit, com, com_type] * m.typeperiod[
                    'weight_typeperiod'][(stf, tm)])

```

(continues on next page)

(continued from previous page)

```

total_consumption *= m.weight
return (total_consumption <=
        m.commodity_dict['max'][(stf, sit, com, com_type)])

```

Sell Per Step Rule: The constraint sell per step rule applies only for commodities of type “Sell” ($c \in C_{\text{sell}}$). This constraint limits the amount of sell commodity $c \in C_{\text{sell}}$, that can be sold by the energy system in the site v in support timeframe y at the timestep t . The limit is defined by the parameter maximum sell supply limit per hour \bar{g}_{yvc} . To satisfy this constraint, the value of the variable sell commodity source term q_{yvct} must be less than or equal to the value of the parameter maximum sell supply limit per hour \bar{g}_{vc} multiplied with the length of the time steps Δt . The mathematical explanation of this rule is given in [Trading with an external market](#).

In script `BuySellPrice.py` the constraint sell per step rule is defined and calculated by the following code fragment:

```

m.res_sell_step = pyomo.Constraint(
    m.tm, m.com_tuples,
    rule=res_sell_step_rule,
    doc='sell commodity output per step <= commodity.maxperstep')

```

```

def res_sell_step_rule(m, tm, stf, sit, com, com_type):
    if com not in m.com_sell:
        return pyomo.Constraint.Skip
    else:
        return (m.e_co_sell[tm, stf, sit, com, com_type] <=
                m.dt * m.commodity_dict['maxperhour']
                [(stf, sit, com, com_type)])

```

Total Sell Rule: The constraint total sell rule applies only for commodities of type “Sell” ($c \in C_{\text{sell}}$). This constraint limits the amount of sell commodity $c \in C_{\text{sell}}$, that can be sold annually by the energy system in the site v and support timeframe y . The limit is defined by the parameter maximum annual sell supply limit per vertex \bar{G}_{yvc} . The annual usage of sell commodity is calculated by the sum of the products of the parameter weight w and the parameter sell commodity source term q_{yvct} , summed over all timesteps $t \in T_m$. The mathematical explanation of this rule is given in [Trading with an external market](#).

In script `BuySellPrice.py` the constraint total sell rule is defined and calculated by the following code fragment:

```

m.res_sell_total = pyomo.Constraint(
    m.com_tuples,
    rule=res_sell_total_rule,
    doc='total sell commodity output <= commodity.max')

```

```

def res_sell_total_rule(m, stf, sit, com, com_type):
    if com not in m.com_sell:
        return pyomo.Constraint.Skip
    else:
        # calculate total sale of commodity com
        total_consumption = 0
        for tm in m.tm:
            total_consumption += (
                m.e_co_sell[tm, stf, sit, com, com_type] * m.typeperiod[
                    'weight_typeperiod'][(stf, tm)])

```

(continues on next page)

(continued from previous page)

```

total_consumption *= m.weight
return (total_consumption <=
        m.commodity_dict['max'][(stf, sit, com, com_type)])

```

Buy Per Step Rule: The constraint buy per step rule applies only for commodities of type “Buy” ($c \in C_{\text{buy}}$). This constraint limits the amount of buy commodity $c \in C_{\text{buy}}$, that can be bought by the energy system in the site v in support timeframe y at the timestep t . The limit is defined by the parameter maximum buy supply limit per time step \bar{b}_{yvc} . To satisfy this constraint, the value of the variable buy commodity source term ψ_{yvct} must be less than or equal to the value of the parameter maximum buy supply limit per time step \bar{b}_{vc} , multiplied by the length of the time steps Δt . The mathematical explanation of this rule is given in *Trading with an external market*.

In script `BuySellPrice.py` the constraint buy per step rule is defined and calculated by the following code fragment:

```

m.res_buy_step = pyomo.Constraint(
    m.tm, m.com_tuples,
    rule=res_buy_step_rule,
    doc='buy commodity output per step <= commodity.maxperstep')

```

```

def res_buy_step_rule(m, tm, stf, sit, com, com_type):
    if com not in m.com_buy:
        return pyomo.Constraint.Skip
    else:
        return (m.e_co_buy[tm, stf, sit, com, com_type] <=
                m.dt * m.commodity_dict['maxperhour']
                [(stf, sit, com, com_type)])

```

Total Buy Rule: The constraint total buy rule applies only for commodities of type “Buy” ($c \in C_{\text{buy}}$). This constraint limits the amount of buy commodity $c \in C_{\text{buy}}$, that can be bought annually by the energy system in the site v in support timeframe y . The limit is defined by the parameter maximum annual buy supply limit per vertex \bar{B}_{yvc} . To satisfy this constraint, the annual usage of buy commodity must be less than or equal to the value of the parameter buy supply limit per vertex \bar{B}_{vc} . The annual usage of buy commodity is calculated by the sum of the products of the parameter weight w and the parameter buy commodity source term ψ_{yvct} , summed over all modeled timesteps $t \in T_m$. The mathematical explanation of this rule is given in *Trading with an external market*.

In script `BuySellPrice.py` the constraint total buy rule is defined and calculated by the following code fragment:

```

m.res_buy_total = pyomo.Constraint(
    m.com_tuples,
    rule=res_buy_total_rule,
    doc='total buy commodity output <= commodity.max')

```

```

def res_buy_total_rule(m, stf, sit, com, com_type):
    if com not in m.com_buy:
        return pyomo.Constraint.Skip
    else:
        # calculate total sale of commodity com
        total_consumption = 0
        for tm in m.tm:
            total_consumption += (

```

(continues on next page)

(continued from previous page)

```

        m.e_co_buy[tm, stf, sit, com, com_type] * m.typeperiod[
→ 'weight_typeperiod'][(stf, tm)])
        total_consumption *= m.weight
        return (total_consumption <=
                m.commodity_dict['max'][(stf, sit, com, com_type)])

```

Environmental Output Per Step Rule: The constraint environmental output per step rule applies only for commodities of type “Env” ($c \in C_{\text{env}}$). This constraint limits the amount of environmental commodity $c \in C_{\text{env}}$, that can be released to environment by the energy system in the site v in support timeframe y at the timestep t . The limit is defined by the parameter maximum environmental output per time step \bar{m}_{yvc} . To satisfy this constraint, the negative value of the commodity balance for the given environmental commodity $c \in C_{\text{env}}$ must be less than or equal to the value of the parameter maximum environmental output per time step \bar{m}_{vc} , multiplied by the length of the time steps Δt . The mathematical explanation of this rule is given in [Minimal optimization model](#).

In script `model.py` the constraint environmental output per step rule is defined and calculated by the following code fragment:

```

m.res_env_step = pyomo.Constraint(
    m.tm, m.com_tuples,
    rule=res_env_step_rule,
    doc='environmental output per step <= commodity.maxperstep')

```

```

def res_env_step_rule(m, tm, stf, sit, com, com_type):
    if com not in m.com_env:
        return pyomo.Constraint.Skip
    else:
        environmental_output = - commodity_balance(m, tm, stf, sit, com)
        return (environmental_output <=
                m.dt * m.commodity_dict['maxperhour']
                [(stf, sit, com, com_type)])

```

Total Environmental Output Rule: The constraint total environmental output rule applies only for commodities of type “Env” ($c \in C_{\text{env}}$). This constraint limits the amount of environmental commodity $c \in C_{\text{env}}$, that can be released to environment annually by the energy system in the site v in support timeframe y . The limit is defined by the parameter maximum annual environmental output limit per vertex \bar{M}_{yvc} . To satisfy this constraint, the annual release of environmental commodity must be less than or equal to the value of the parameter maximum annual environmental output \bar{M}_{vc} . The annual release of environmental commodity is calculated by the sum of the products of the parameter weight w and the negative value of commodity balance function, summed over all modeled time steps $t \in T_m$. The mathematical explanation of this rule is given in [Minimal optimization model](#).

In script `model.py` the constraint total environmental output rule is defined and calculated by the following code fragment:

```

m.res_env_total = pyomo.Constraint(
    m.com_tuples,
    rule=res_env_total_rule,
    doc='total environmental commodity output <= commodity.max')

```

```

def res_env_total_rule(m, stf, sit, com, com_type):
    if com not in m.com_env:
        return pyomo.Constraint.Skip

```

(continues on next page)

(continued from previous page)

```

else:
    # calculate total creation of environmental commodity com
    env_output_sum = 0
    for tm in m.tm:
        env_output_sum += (- commodity_balance(m, tm, stf, sit, com) *
    ↪ m.typeperiod['weight_typeperiod'][(stf,tm)])
        env_output_sum *= m.weight
    return (env_output_sum <=
            m.commodity_dict['max'][(stf, sit, com, com_type)])

```

Demand Side Management Constraints

The DSM equations are taken from the Paper of Zerrahn and Schill “On the representation of demand-side management in power system models”, DOI: [10.1016/j.energy.2015.03.037](https://doi.org/10.1016/j.energy.2015.03.037).

DSM Variables Rule: The DSM variables rule defines the relation between the up- and downshifted DSM commodities. An upshift δ_{yvc}^{up} in site v and support timeframe y of demand commodity c in time step t can be compensated during a certain time step interval $[t - y_{yvc}/\Delta t, t + y_{yvc}/\Delta t]$ by multiple downshifts $\delta_{t,tt,yvc}^{\text{down}}$. Here, y_{yvc} represents the allowable delay time of downshifts in hours, which is scaled into time steps by dividing by the timestep length Δt . Depending on the DSM efficiency e_{yvc} , an upshift in a DSM commodity may correspond to multiple downshifts which sum to less than the original upshift. The mathematical explanation of this rule is given in *Demand side management*.

In script `dsm.py` the constraint DSM variables rule is defined by the following code fragment:

```

m.def_dsm_variables = pyomo.Constraint(
    m.tm, m.dsm_site_tuples,
    rule=def_dsm_variables_rule,
    doc='DSMup * efficiency factor n == DSMdo (summed)')

```

```

def def_dsm_variables_rule(m, tm, stf, sit, com):
    dsm_down_sum = 0
    for tt in dsm_time_tuples(tm,
                               m.timesteps[1:],
                               max(int(1 / m.dt *
    ↪ m.dsm_dict['delay'][(stf, sit, com)]),
    ↪ 1)):
        dsm_down_sum += m.dsm_down[tm, tt, stf, sit, com]
    return dsm_down_sum == (m.dsm_up[tm, stf, sit, com] *
                            m.dsm_dict['eff'][(stf, sit, com)])

```

DSM Upward Rule: The DSM upshift δ_{yvc}^{up} in site v and support timeframe y of demand commodity c in time step t is limited by the DSM maximal upshift per hour $\bar{K}_{yvc}^{\text{up}}$, multiplied by the length of the time steps Δt . The mathematical explanation of this rule is given in *Demand side management*.

In script `dsm.py` the constraint DSM upward rule is defined by the following code fragment:

```

m.res_dsm_upward = pyomo.Constraint(
    m.tm, m.dsm_site_tuples,
    rule=res_dsm_upward_rule,
    doc='DSMup <= Cup (threshold capacity of DSMup)')

```

```
def res_dsm_upward_rule(m, tm, stf, sit, com):
    return m.dsm_up[tm, stf, sit, com] <= (m.dt *
                                             m.dsm_dict['cap-max-up']
                                             [(stf, sit, com)])
```

DSM Downward Rule: The total DSM downshift $\delta_{t,tt,yvc}^{\text{down}}$ in site v and support timeframe y of demand commodity c in time step t is limited by the DSM maximal downshift per hour $\bar{K}_{yvc}^{\text{down}}$, multiplied by the length of the time steps Δt . The mathematical explanation of this rule is given in [Demand side management](#).

In script `dsm.py` the constraint DSM downward rule is defined by the following code fragment:

```
m.res_dsm_downward = pyomo.Constraint(
    m.tm, m.dsm_site_tuples,
    rule=res_dsm_downward_rule,
    doc='DSMdo (summed) <= Cdo (threshold capacity of DSMdo)')
```

```
def res_dsm_downward_rule(m, tm, stf, sit, com):
    dsm_down_sum = 0
    for t in dsm_time_tuples(tm,
                              m.timesteps[1:],
                              max(int(1 / m.dt *
                                      m.dsm_dict['delay'][(stf, sit, com)]),
    ↪1)):
        dsm_down_sum += m.dsm_down[t, tm, stf, sit, com]
    return dsm_down_sum <= (m.dt * m.dsm_dict['cap-max-do'][(stf, sit,
    ↪com)])
```

DSM Maximum Rule: The DSM maximum rule limits the shift of one DSM unit in site v in support timeframe y of demand commodity c in time step t . The mathematical explanation of this rule is given in [Demand side management](#).

In script `dsm.py` the constraint DSM maximum rule is defined by the following code fragment:

```
m.res_dsm_maximum = pyomo.Constraint(
    m.tm, m.dsm_site_tuples,
    rule=res_dsm_maximum_rule,
    doc='DSMup + DSMdo (summed) <= max(Cup,Cdo)')
```

```
def res_dsm_maximum_rule(m, tm, stf, sit, com):
    dsm_down_sum = 0
    for t in dsm_time_tuples(tm,
                              m.timesteps[1:],
                              max(int(1 / m.dt *
                                      m.dsm_dict['delay'][(stf, sit, com)]),
    ↪1)):
        dsm_down_sum += m.dsm_down[t, tm, stf, sit, com]

    max_dsm_limit = m.dt * max(m.dsm_dict['cap-max-up'][(stf, sit, com)],
                               m.dsm_dict['cap-max-do'][(stf, sit, com)])
    return m.dsm_up[tm, stf, sit, com] + dsm_down_sum <= max_dsm_limit
```

DSM Recovery Rule: The DSM recovery rule limits the upshift in site v and support timeframe y of demand commodity c during a set recovery period o_{yvc} . Since the recovery period o_{yvc} is input as hours, it is scaled into time steps by dividing it by the length of the time steps Δt . The mathematical explanation of this rule is given in [Demand side management](#).

In script `dsm.py` the constraint DSM Recovery rule is defined by the following code fragment:

```
m.res_dsm_recovery = pyomo.Constraint(
    m.tm, m.dsm_site_tuples,
    rule=res_dsm_recovery_rule,
    doc='DSMup(t, t + recovery time R) <= Cup * delay time L')

def res_dsm_recovery_rule(m, tm, stf, sit, com):
    dsm_up_sum = 0
    for t in dsm_recovery(tm,
                           m.timesteps[1:],
                           max(int(1 / m.dt *
                                   m.dsm_dict['recov'][(stf, sit, com)]), 1)):
        dsm_up_sum += m.dsm_up[t, stf, sit, com]
    return dsm_up_sum <= (m.dsm_dict['cap-max-up'][(stf, sit, com)] *
                           m.dsm_dict['delay'][(stf, sit, com)])
```

Global Environmental Constraint

Global CO2 Limit Rule: The constraint global CO2 limit rule applies to the whole energy system in one support timeframe y , that is to say it applies to every site and timestep. This constraints restricts the total amount of CO2 to environment. The constraint states that the sum of released CO2 across all sites $v \in V$ and timesteps $t \in t_m$ must be less than or equal to the parameter maximum global annual CO2 emission limit $\bar{L}_{CO_2,y}$, where the amount of released CO2 in a single site v at a single timestep t is calculated by the product of commodity balance of environmental commodities $CB(y, v, CO_2, t)$ and the parameter weight w . This constraint is skipped if the value of the parameter \bar{L}_{CO_2} is set to `inf`. The mathematical explanation of this rule is given in [Minimal optimization model](#).

In script `model.py` the constraint annual global CO2 limit rule is defined and calculated by the following code fragment:

```
def res_global_co2_limit_rule(m, stf):
    if math.isinf(m.global_prop_dict['value'][stf, 'CO2 limit']):
        return pyomo.Constraint.Skip
    elif m.global_prop_dict['value'][stf, 'CO2 limit'] >= 0:
        co2_output_sum = 0
        for tm in m.tm:
            for sit in m.sit:
                # minus because negative commodity_balance represents_
                ↪ creation
                # of that commodity.
                co2_output_sum += (- commodity_balance(m, tm, stf, sit,
                ↪ 'CO2') * m.typeperiod['weight_typeperiod'][(stf,tm)])

                # scaling to annual output (cf. definition of m.weight)
                co2_output_sum *= m.weight
            return (co2_output_sum <= m.global_prop_dict['value']
                    [stf, 'CO2 limit'])
    else:
        return pyomo.Constraint.Skip
```

Global CO2 Budget Rule: The constraint global CO2 budget rule applies to the whole energy system over the entire modeling horizon, that is to say it applies to every support timeframe, site and timestep. This constraints restricts the total amount of CO2 to environment. The constraint states that the sum of

released CO₂ across all support timeframe $y \in Y$, sites $v \in V$ and timesteps $t \in t_m$ must be less than or equal to the parameter maximum global CO₂ emission budget $\bar{L}_{CO_2,y}$, where the amount of released CO₂ in a single support timeframe y in a single site v and at a single timestep t is calculated by the product of the commodity balance of environmental commodities $CB(y, v, CO_2, t)$ and the parameter weight w . This constraint is skipped if the value of the parameter \bar{L}_{CO_2} is set to `inf`. The mathematical explanation of this rule is given in *Intertemporal optimization model*.

In script `model.py` the constraint global CO₂ budget is defined and calculated by the following code fragment:

```
def res_global_co2_budget_rule(m):
    if math.isinf(m.global_prop_dict['value'][min(m.stf_list), 'CO2 budget
    →']):
        return pyomo.Constraint.Skip
    elif (m.global_prop_dict['value'][min(m.stf_list), 'CO2 budget']) >= 0:
        co2_output_sum = 0
        for stf in m.stf:
            for tm in m.tm:
                for sit in m.sit:
                    # minus because negative commodity_balance represents
                    # creation of that commodity.
                    co2_output_sum += (- commodity_balance
                                     (m, tm, stf, sit, 'CO2') *
                                     m.typeperiod['weight_typeperiod
    →'][(stf,tm)] *
                                     m.weight *
                                     stf_dist(stf, m))

        return (co2_output_sum <=
                m.global_prop_dict['value'][min(m.stf), 'CO2 budget'])
    else:
        return pyomo.Constraint.Skip
```

Process Constraints

Process Capacity Rule: The constraint process capacity rule defines the variable total process capacity κ_{yvp} . The variable total process capacity is defined by the constraint as the sum of the parameter process capacity installed K_{vp} and the variable new process capacity $\hat{\kappa}_{yvp}$. The mathematical explanation of this rule is given in *Minimal optimization model*.

In script `model.py` the constraint process capacity rule is defined and calculated by the following code fragment:

```
m.def_process_capacity = pyomo.Constraint(
    m.pro_tuples,
    rule=def_process_capacity_rule,
    doc='total process capacity = inst-cap + new capacity')

def def_process_capacity_rule(m, stf, sit, pro):
    if m.mode['int']:
        if (sit, pro, stf) in m.inst_pro_tuples:
            if (sit, pro, min(m.stf)) in m.pro_const_cap_dict:
                cap_pro = m.process_dict['inst-cap'][(stf, sit, pro)]
            else:
```

(continues on next page)

(continued from previous page)

```

        cap_pro = \
            (sum(m.cap_pro_new[stf_built, sit, pro]
                 for stf_built in m.stf
                 if (sit, pro, stf_built, stf)
                 in m.operational_pro_tuples) +
             m.process_dict['inst-cap'][(min(m.stf), sit, pro)])
    else:
        cap_pro = sum(
            m.cap_pro_new[stf_built, sit, pro]
            for stf_built in m.stf
            if (sit, pro, stf_built, stf) in m.operational_pro_tuples)
    else:
        if (sit, pro, stf) in m.pro_const_cap_dict:
            cap_pro = m.process_dict['inst-cap'][(stf, sit, pro)]
        else:
            cap_pro = (m.cap_pro_new[stf, sit, pro] +
                       m.process_dict['inst-cap'][(stf, sit, pro)])
    return cap_pro

```

Process Input Rule: The constraint process input rule defines the variable process input commodity flow $\epsilon_{yvcpt}^{\text{in}}$. The variable process input commodity flow is defined by the constraint as the product of the variable process throughput τ_{yvpt} and the parameter process input ratio r_{ypc}^{in} . The mathematical explanation of this rule is given in *Minimal optimization model*.

In script `model.py` the constraint process input rule is defined and calculated by the following code fragment:

```

m.def_process_input = pyomo.Constraint(
    m.tm, m.pro_input_tuples - m.pro_partial_input_tuples,
    rule=def_process_input_rule,
    doc='process input = process throughput * input ratio')

```

```

def def_process_input_rule(m, tm, stf, sit, pro, com):
    return (m.e_pro_in[tm, stf, sit, pro, com] ==
            m.tau_pro[tm, stf, sit, pro] * m.r_in_dict[(stf, pro, com)])

```

Process Output Rule: The constraint process output rule defines the variable process output commodity flow $\epsilon_{yvcpt}^{\text{out}}$. The variable process output commodity flow is defined by the constraint as the product of the variable process throughput τ_{yvpt} and the parameter process output ratio r_{ypc}^{out} . The mathematical explanation of this rule is given in *Minimal optimization model*.

In script `model.py` the constraint process output rule is defined and calculated by the following code fragment:

```

m.def_process_output = pyomo.Constraint(
    m.tm, (m.pro_output_tuples - m.pro_partial_output_tuples -
           m.pro_timevar_output_tuples),
    rule=def_process_output_rule,
    doc='process output = process throughput * output ratio')

```

```

def def_process_output_rule(m, tm, stf, sit, pro, com):
    if com == 'electricity-reactive':
        return pyomo.Constraint.Skip
    else:

```

(continues on next page)

(continued from previous page)

```

return (m.e_pro_out[tm, stf, sit, pro, com] ==
        m.tau_pro[tm, stf, sit, pro] * m.r_out_dict[(stf, pro, com)])

```

Intermittent Supply Rule: The constraint intermittent supply rule defines the variable process input commodity flow $\epsilon_{yvcp}^{\text{in}}$ for processes p that use a supply intermittent commodity $c \in C_{\text{sup}}$ as input. Therefore this constraint only applies if a commodity is an intermittent supply commodity $c \in C_{\text{sup}}$. The variable process input commodity flow is defined by the constraint as the product of the variable total process capacity κ_{yvp} and the parameter intermittent supply capacity factor s_{yvct} , scaled by the size of the time steps :math: Delta t. The mathematical explanation of this rule is given in [Minimal optimization model](#).

In script `model.py` the constraint intermittent supply rule is defined and calculated by the following code fragment:

```

m.def_intermittent_supply = pyomo.Constraint(
    m.tm, m.pro_input_tuples,
    rule=def_intermittent_supply_rule,
    doc='process output = process capacity * supim timeseries')

```

```

def def_intermittent_supply_rule(m, tm, stf, sit, pro, coin):
    if coin in m.com_supim:
        return (m.e_pro_in[tm, stf, sit, pro, coin] ==
                m.cap_pro[stf, sit, pro] * m.supim_dict[(sit, coin)]
                [(stf, tm)] * m.dt)
    else:
        return pyomo.Constraint.Skip

```

Process Throughput By Capacity Rule: The constraint process throughput by capacity rule limits the variable process throughput τ_{yvpt} . This constraint prevents processes from exceeding their capacity. The constraint states that the variable process throughput must be less than or equal to the variable total process capacity κ_{yvp} , scaled by the size of the time steps :math: Delta t. The mathematical explanation of this rule is given in [Minimal optimization model](#).

In script `model.py` the constraint process throughput by capacity rule is defined and calculated by the following code fragment:

```

m.res_process_throughput_by_capacity = pyomo.Constraint(
    m.tm, m.pro_tuples,
    rule=res_process_throughput_by_capacity_rule,
    doc='process throughput <= total process capacity')

```

```

def res_process_throughput_by_capacity_rule(m, tm, stf, sit, pro):
    return (m.tau_pro[tm, stf, sit, pro] <= m.dt * m.cap_pro[stf, sit,
    ↪pro])

```

Process Throughput Gradient Rule: The constraint process throughput gradient rule limits the process power gradient $|\tau_{yvpt} - \tau_{yvpt(t-1)}|$. This constraint prevents processes from exceeding their maximal possible change in activity from one time step to the next. The constraint states that the absolute power gradient must be less than or equal to the maximal power ramp up gradient $\overline{PG}_{yvp}^{\text{up}}$ parameter when increasing power or to the maximal power ramp down gradient $\overline{PG}_{yvp}^{\text{up}}$ parameter (both scaled to capacity and by time step duration). The mathematical explanation of this rule is given in [Minimal optimization model](#).

In script `model.py` the constraint process throughput gradient rule is split into 2 parts and defined and

calculated by the following code fragments:

```
m.res_process_rampdown = pyomo.Constraint(
    m.tm, m.pro_rampdowngrad_tuples,
    rule=res_process_rampdown_rule,
    doc='throughput may not decrease faster than maximal ramp down gradient
↪')
m.res_process_rampup = pyomo.Constraint(
    m.tm, m.pro_rampupgrad_tuples,
    rule=res_process_rampup_rule,
    doc='throughput may not increase faster than maximal ramp up gradient')
```

```
def res_process_rampdown_rule(m, t, stf, sit, pro):
    return (m.tau_pro[t - 1, stf, sit, pro] -
            m.cap_pro[stf, sit, pro] *
            m.process_dict['ramp-down-grad'][(stf, sit, pro)] * m.dt <=
            m.tau_pro[t, stf, sit, pro])
```

```
def res_process_rampup_rule(m, t, stf, sit, pro):
    return (m.tau_pro[t - 1, stf, sit, pro] +
            m.cap_pro[stf, sit, pro] *
            m.process_dict['ramp-up-grad'][(stf, sit, pro)] * m.dt >=
            m.tau_pro[t, stf, sit, pro])
```

Process Capacity Limit Rule: The constraint process capacity limit rule limits the variable total process capacity κ_{yvp} . This constraint restricts a process p in a site v and support timeframe y from having more total capacity than an upper bound and having less than a lower bound. The constraint states that the variable total process capacity κ_{yvp} must be greater than or equal to the parameter process capacity lower bound \underline{K}_{yvp} and less than or equal to the parameter process capacity upper bound \overline{K}_{yvp} . The mathematical explanation of this rule is given in *Minimal optimization model*.

In script `model.py` the constraint process capacity limit rule is defined and calculated by the following code fragment:

```
m.res_process_capacity = pyomo.Constraint(
    m.pro_tuples,
    rule=res_process_capacity_rule,
    doc='process.cap-lo <= total process capacity <= process.cap-up')
```

```
def res_process_capacity_rule(m, stf, sit, pro):
    return (m.process_dict['cap-lo'][stf, sit, pro],
            m.cap_pro[stf, sit, pro],
            m.process_dict['cap-up'][stf, sit, pro])
```

Sell Buy Symmetry Rule: The constraint sell buy symmetry rule defines the total process capacity κ_{yvp} of a process p in a site v and support timeframe y that uses either sell or buy commodities ($c \in C_{\text{sell}} \vee C_{\text{buy}}$), therefore this constraint only applies to processes that use sell or buy commodities. The constraint states that the total process capacities κ_{yvp} of processes that use complementary buy and sell commodities must be equal. Buy and sell commodities are complementary, when a commodity c is an output of a process where the buy commodity is an input, and at the same time the commodity c is an input commodity of a process where the sell commodity is an output. The mathematical explanation of this rule is given in *Trading with an external market*.

In script `BuySellPrice.py` the constraint sell buy symmetry rule is defined and calculated by the following code fragment:

```
m.res_sell_buy_symmetry = pyomo.Constraint(
    m.pro_input_tuples,
    rule=res_sell_buy_symmetry_rule,
    doc='total power connection capacity must be symmetric in both '
        'directions')
```

```
def res_sell_buy_symmetry_rule(m, stf, sit_in, pro_in, coin):
    # constraint only for sell and buy processes
    # and the processes must be in the same site
    if coin in m.com_buy:
        sell_pro = search_sell_buy_tuple(m, stf, sit_in, pro_in, coin)
        if sell_pro is None:
            return pyomo.Constraint.Skip
        else:
            return (m.cap_pro[stf, sit_in, pro_in] ==
                    m.cap_pro[stf, sit_in, sell_pro])
    else:
        return pyomo.Constraint.Skip
```

Process time variable output rule: This constraint multiplies the process efficiency with the parameter time series f_{yvpt}^{out} . The process output for all commodities is thus manipulated depending on time. This constraint is not valid for environmental commodities since these are typically linked to an input commodity flow rather than an output commodity flow. The mathematical explanation of this rule is given in *Advanced Processes*.

In script `AdvancedProcesses.py` the constraint process time variable output rule is defined and calculated by the following code fragment:

```
m.def_process_timevar_output = pyomo.Constraint(
    m.tm, m.pro_timevar_output_tuples,
    rule=def_pro_timevar_output_rule,
    doc='e_pro_out = tau_pro * r_out * eff_factor')
```

```
def def_pro_timevar_output_rule(m, tm, stf, sit, pro, com):
    return (m.e_pro_out[tm, stf, sit, pro, com] ==
            m.tau_pro[tm, stf, sit, pro] * m.r_out_dict[(stf, pro, com)] *
            m.eff_factor_dict[(sit, pro)][stf, tm])
```

Process Constraints for partial operation

The process constraints for partial operation described in the following are only activated if in the input file there is a value set in the column **ratio-min** for an **input commodity** or for an **output commodity** in the **process-commodity** sheet for the process in question.

It is important to understand that this partial load formulation can only work if its accompanied by a non-zero value for the minimum partial load fraction \underline{P}_{yvp} .

Without activating the on/off feature in the **process** sheet, the partial load feature can only be used for processes that are never meant to be shut down and are always operating only between a given part load state and full load. Please see the next chapter for the combined on/off and partial operation features.

Throughput by Min fraction Rule: This constraint limits the minimal operational state of a process downward, making sure that the minimal part load fraction is honored. The mathematical explanation of this rule is given in *Advanced Processes*.

In script `AdvancedProcesses.py` this constraint is defined and calculated by the following code fragment:

```
m.res_throughput_by_capacity_min = pyomo.Constraint(
    m.tm, m.pro_partial_tuples,
    rule=res_throughput_by_capacity_min_rule,
    doc='cap_pro * min-fraction <= tau_pro')
```

```
def res_throughput_by_capacity_min_rule(m, tm, stf, sit, pro):
    return (m.tau_pro[tm, stf, sit, pro] >=
            m.cap_pro[stf, sit, pro] *
            m.process_dict['min-fraction'][(stf, sit, pro)] * m.dt)
```

Partial Process Input Rule: The link between operational state τ_{yvp} and commodity in/outputs is changed from a simple linear behavior to a more complex one. Instead of constant in- and output ratios these are now interpolated linearly between the value for full operation $r_{yvp}^{in/out}$ at full load and the minimum in/output ratios $r_{yvp}^{in/out}$ at the minimum operation point. The mathematical explanation of this rule is given in *Advanced Processes*.

In script `model.py` this expression is written in the following way for the input ratio (and analogous for the output ratios):

```
m.def_partial_process_input = pyomo.Constraint(
    m.tm, m.pro_partial_input_tuples,
    rule=def_partial_process_input_rule,
    doc='e_pro_in = cap_pro * min_fraction * (r - R) / (1 - min_fraction)'
        '+ tau_pro * (R - min_fraction * r) / (1 - min_fraction)')
```

```
def def_partial_process_input_rule(m, tm, stf, sit, pro, com):
    # input ratio at maximum operation point
    R = m.r_in_dict[(stf, pro, com)]
    # input ratio at lowest operation point
    r = m.r_in_min_fraction_dict[(stf, pro, com)]
    min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]

    online_factor = min_fraction * (r - R) / (1 - min_fraction)
    throughput_factor = (R - min_fraction * r) / (1 - min_fraction)
    return (m.e_pro_in[tm, stf, sit, pro, com] ==
            m.dt * m.cap_pro[stf, sit, pro] * online_factor +
            m.tau_pro[tm, stf, sit, pro] * throughput_factor)
```

In case of a process where also a time variable output efficiency is given the code for the output changes to.

```
m.def_process_partial_timevar_output = pyomo.Constraint(
    m.tm, m.pro_partial_output_tuples & m.pro_timevar_output_tuples,
    rule=def_pro_partial_timevar_output_rule,
    doc='e_pro_out = tau_pro * r_out * eff_factor')
```

```
def def_pro_partial_timevar_output_rule(m, tm, stf, sit, pro, com):
    # input ratio at maximum operation point
    R = m.r_out_dict[(stf, pro, com)]
    # input ratio at lowest operation point
    r = m.r_out_min_fraction_dict[(stf, pro, com)]
    min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]
```

(continues on next page)

(continued from previous page)

```

online_factor = min_fraction * (r - R) / (1 - min_fraction)
throughput_factor = (R - min_fraction * r) / (1 - min_fraction)
return (m.e_pro_out[tm, stf, sit, pro, com] ==
        (m.dt * m.cap_pro[stf, sit, pro] * online_factor +
         m.tau_pro[tm, stf, sit, pro] * throughput_factor) *
        m.eff_factor_dict[(sit, pro)][stf, tm])

```

Process Constraints for the on/off feature

The process constraints for the on/off feature described in this chapter are only activated if, in the input file, the value „1” is set in the column **on-off** for a process in the **process** sheet.

Process Throughput and On/Off Coupling Rule: These two constraints couple the variables process throughput τ_{yvpt} and process on/off marker y_{vpt} . This is done by turning the marker on (boolean value 1) when the throughput is greater than the minimum load of the process. The mathematical explanation of this rule is given in [Advanced Processes](#).

In script `AdvancedProcesses.py` this constraint is defined and calculated by the following code fragment:

```

m.res_throughput_by_on_off_lower = pyomo.Constraint(
    m.tm, m.pro_on_off_tuples | m.pro_partial_on_off_tuples,
    rule=res_throughput_by_on_off_lower_rule,
    doc='tau_pro >= min-fraction * cap_pro * on_off')
m.res_throughput_by_on_off_upper = pyomo.Constraint(
    m.tm, m.pro_on_off_tuples | m.pro_partial_on_off_tuples,
    rule=res_throughput_by_on_off_upper_rule,
    doc='tau_pro <='
        'cap_pro * on_off + min-fraction * cap_pro * (1 - on_off)')

```

```

def res_throughput_by_on_off_lower_rule(m, tm, stf, sit, pro):
    return (m.tau_pro[tm, stf, sit, pro] >=
            m.min_fraction_dict[stf, sit, pro] * m.cap_pro[stf, sit, pro] *
            m.dt * m.on_off[tm, stf, sit, pro])

```

```

def res_throughput_by_on_off_upper_rule(m, tm, stf, sit, pro):
    return (m.tau_pro[tm, stf, sit, pro] <=
            m.cap_pro[stf, sit, pro] * m.dt * m.on_off[tm, stf, sit, pro] +
            m.min_fraction_dict[stf, sit, pro] * m.cap_pro[stf, sit, pro] *
            m.dt * (1 - m.on_off[tm, stf, sit, pro]))

```

Process On/Off Output Rule: This constraint modifies the process output commodity flow $\epsilon_{yvcp}^{\text{out}}$ when compared to the original version without the on/off feature in two ways by differentiating between the output **commodity type** q . When the **commodity type** is Env, the output remains the same as without the on/off feature. Otherwise, the original output equation is multiplied with the variable process on/off marker y_{vpt} . The mathematical explanation of this rule is given in [Advanced Processes](#).

In script `AdvancedProcesses.py` the constraint process on/off output rule is defined and calculated by the following code fragment:

```
m.def_process_on_off_output = pyomo.Constraint(
    m.tm, m.pro_on_off_output_tuples - m.pro_timevar_output_tuples -
        m.pro_partial_on_off_output_tuples,
    rule=def_process_on_off_output_rule,
    doc='e_pro_out = tau_pro * r_out * on_off')
```

```
def def_process_on_off_output_rule(m, tm, stf, sit, pro, com):
    r = m.r_out_dict[(stf, pro, com)]
    if com in m.com_env:
        return (m.e_pro_out[tm, stf, sit, pro, com] ==
                m.tau_pro[tm, stf, sit, pro] * r)
    else:
        return (m.e_pro_out[tm, stf, sit, pro, com] ==
                m.tau_pro[tm, stf, sit, pro] * r * m.on_off[tm, stf, sit,
↪pro])
```

In the case of a process where also a time variable output efficiency is given the code for the output changes to:

```
m.def_process_on_off_timevar_output = pyomo.Constraint(
    m.tm, m.pro_timevar_output_tuples & m.pro_on_off_output_tuples -
        m.pro_partial_on_off_output_tuples,
    rule=def_process_on_off_timevar_output_rule,
    doc='e_pro_out == tau_pro * r_out * on_off * eff_factor')
```

```
def def_process_on_off_timevar_output_rule(m, tm, stf, sit, pro, com):
    return (m.e_pro_out[tm, stf, sit, pro, com] ==
            m.tau_pro[tm, stf, sit, pro] * m.r_out_dict[(stf, pro, com)] *
            m.on_off[tm, stf, sit, pro] *
            m.eff_factor_dict[(sit, pro)][stf, tm])
```

Process On/Off Partial Input Rule: This constraint modifies the process input commodity flow $\epsilon_{yvpt}^{\text{in}}$ when compared to the original partial operation version without the on/off feature in by differentiating between two possible input functions, depending on the process on/off marker y_{vpt} . When the marker is on, the input function is the same as in the case of simple partial operation. When the marker is off, the input function becomes the product of the variable process throughput τ_{yvpt} and the parameter process partial input ratio r_{ypc}^{in} . the output **commodity type** q . When the **commodity type**. The mathematical explanation of this rule is given in *Advanced Processes*.

In script `AdvancedProcesses.py` the constraint process on/off output rule is defined and calculated by the following code fragment:

```
m.def_partial_process_on_off_input = pyomo.Constraint(
    m.tm, m.pro_partial_on_off_input_tuples,
    rule=def_partial_process_on_off_input_rule,
    doc='e_pro_in = '
        ' (cap_pro * min_fraction * (r - R) / (1 - min_fraction))'
        ' + tau_pro * (R - min_fraction * r) / (1 - min_fraction))')
```

```
def def_partial_process_on_off_input_rule(m, tm, stf, sit, pro, com):
    # input ratio at maximum operation point
    R = m.r_in_dict[(stf, pro, com)]
    # input ratio at lowest operation point
    r = m.r_in_min_fraction_dict[stf, pro, com]
```

(continues on next page)

(continued from previous page)

```
min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]

online_factor = min_fraction * (r - R) / (1 - min_fraction)
throughput_factor = (R - min_fraction * r) / (1 - min_fraction)
return (m.e_pro_in[tm, stf, sit, pro, com] ==
        (m.dt * m.cap_pro[stf, sit, pro] * online_factor +
         m.tau_pro[tm, stf, sit, pro] * throughput_factor) *
         m.on_off[tm, stf, sit, pro] +
         m.tau_pro[tm, stf, sit, pro] * r *
         (1 - m.on_off[tm, stf, sit, pro])))
```

Process On/Off Partial Output Rule: This constraint modifies the process output commodity flow $\epsilon_{yvpt}^{\text{out}}$ when compared to the original partial operation version without the on/off feature in two ways by differentiating between the output **commodity type** q . When the **commodity type** is not Env, the output remains the same as for the partial operation without the on/off feature. Otherwise, the original output equation is changes depending on the variable process on/off marker $yvpt$. When the marker is off, the output function becomes the product of the variable process throughput τ_{yvpt} and the parameter process partial output ratio r_{ypc}^{out} . When the marker is on, the output function for Env type commodities remains the same as for the partial operation without the on/off feature. The mathematical explanation of this rule is given in [Advanced Processes](#).

```
m.def_partial_process_on_off_output = pyomo.Constraint(
    m.tm, m.pro_partial_on_off_output_tuples - m.pro_timevar_output_tuples,
    rule=def_partial_process_on_off_output_rule,
    doc='e_pro_out = on_off * '
        ' (cap_pro * min_fraction * (r - R) / (1 - min_fraction) '
        '+ tau_pro * (R - min_fraction * r) / (1 - min_fraction)) ')
```

```
def def_partial_process_on_off_output_rule(m, tm, stf, sit, pro, com):
    # input ratio at maximum operation point
    R = m.r_out_dict[stf, pro, com]
    # input ratio at lowest operation point
    r = m.r_out_min_fraction_dict[stf, pro, com]
    min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]
    on_off = m.on_off[tm, stf, sit, pro]

    online_factor = min_fraction * (r - R) / (1 - min_fraction)
    throughput_factor = (R - min_fraction * r) / (1 - min_fraction)
    if com in m.com_env:
        return (m.e_pro_out[tm, stf, sit, pro, com] ==
                (m.dt * m.cap_pro[stf, sit, pro] * online_factor +
                 m.tau_pro[tm, stf, sit, pro] * throughput_factor) * on_off +
                 m.tau_pro[tm, stf, sit, pro] * r *
                 (1 - on_off))
    else:
        return (m.e_pro_out[tm, stf, sit, pro, com] ==
                (m.dt * m.cap_pro[stf, sit, pro] * online_factor +
                 m.tau_pro[tm, stf, sit, pro] * throughput_factor) * on_off)
```

In the case of a process where also a time variable output efficiency is given the code for the output changes to:

```
m.def_process_partial_on_off_timevar_output = pyomo.Constraint(
    m.tm, m.pro_partial_on_off_output_tuples & m.pro_timevar_output_tuples,
```

(continues on next page)

(continued from previous page)

```
rule=def_pro_partial_on_off_timevar_output_rule,
doc='e_pro_out == tau_pro * r_out * on_off * eff_factor')
```

```
def def_partial_process_on_off_output_rule(m, tm, stf, sit, pro, com):
    # input ratio at maximum operation point
    R = m.r_out_dict[stf, pro, com]
    # input ratio at lowest operation point
    r = m.r_out_min_fraction_dict[stf, pro, com]
    min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]
    on_off = m.on_off[tm, stf, sit, pro]

    online_factor = min_fraction * (r - R) / (1 - min_fraction)
    throughput_factor = (R - min_fraction * r) / (1 - min_fraction)
    if com in m.com_env:
        return (m.e_pro_out[tm, stf, sit, pro, com] ==
                (m.dt * m.cap_pro[stf, sit, pro] * online_factor +
                 m.tau_pro[tm, stf, sit, pro] * throughput_factor) * on_off +
                 m.tau_pro[tm, stf, sit, pro] * r *
                 (1 - on_off))
    else:
        return (m.e_pro_out[tm, stf, sit, pro, com] ==
                (m.dt * m.cap_pro[stf, sit, pro] * online_factor +
                 m.tau_pro[tm, stf, sit, pro] * throughput_factor) * on_off)
```

Process Starting Ramp-up Rule: This constraint replaces the process throughput ramping rule when the parameter process starting time $\overline{ST}_{yvp}^{\text{start}}$ is defined in the input **process** sheet. This is done only until the variable process throughput τ_{yvp} reaches the minimum load value and only while increasing the process throughput τ_{yvp} . The mathematical explanation of this rule is given in [Advanced Processes](#).

In script `AdvancedProcesses.py` the constraint process starting ramp-up rule is defined and calculated by the following code fragment:

```
m.res_starting_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_start_tuples,
    rule=res_starting_rampup_rule,
    doc='throughput may not increase faster than maximal starting ramp up '
        'gradient until reaching minimum capacity')
```

```
def res_starting_rampup_rule(m, t, stf, sit, pro):
    min_fraction = m.min_fraction_dict[stf, sit, pro]
    start_time = m.process_dict['start-time'][(stf, sit, pro)]
    starting_ramp = min_fraction / start_time
    return (m.tau_pro[t - 1, stf, sit, pro] +
            m.cap_pro[stf, sit, pro] *
            m.process_dict['ramp-up-grad'][(stf, sit, pro)] * m.dt *
            m.on_off[t - 1, stf, sit, pro] +
            m.cap_pro[stf, sit, pro] *
            starting_ramp * m.dt *
            (1 - m.on_off[t - 1, stf, sit, pro]))
    >=
    m.tau_pro[t, stf, sit, pro])
```

Process Output Ramping Rule: These constraints act as a limiter for the process output $\epsilon_{yvp}^{\text{out}}$ with the on/off feature because the process on/off marker y_{vp} can be both on and off in the minimum load point. There are three possible cases, as follows, defined in the script `AdvanceProcesses.py`. The

mathematical explanation of this rule is given in *Advanced Processes*

Case I: The parameter process minimum load fraction \underline{P}_{yvp} is greater than the parameter process maximum power ramp up gradient $\overline{PG}_{yvp}^{\text{up}}$ and is divisible with it. It is defined and calculated by the following code fragment:

```
m.res_output_minfraction_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_divides_minfraction_output_tuples -
        m.pro_partial_on_off_output_tuples - m.pro_timevar_output_tuples,
    rule=res_output_minfraction_rampup_rule,
    doc='Output may not increase faster than the minimal working capacity')
```

```
def res_output_minfraction_rampup_rule(m, tm, stf, sit, pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                m.process_dict['min-fraction'][(stf, sit, pro)] *
                m.r_out_dict[(stf, pro, com)] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip
```

If the process has partial operation, the code changes to:

```
m.res_partial_output_minfraction_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_divides_minfraction_output_tuples &
        m.pro_partial_on_off_output_tuples - m.pro_timevar_output_tuples,
    rule=res_partial_output_minfraction_rampup_rule,
    doc='Output may not increase faster than the minimal working capacity')
```

```
def res_partial_output_minfraction_rampup_rule(m, tm, stf, sit, pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                m.process_dict['min-fraction'][(stf, sit, pro)] *
                m.r_out_min_fraction_dict[(stf, pro, com)] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip
```

If the process has time variable efficiency, the code changes to:

```
m.res_timevar_output_minfraction_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_divides_minfraction_output_tuples &
        m.pro_timevar_output_tuples - m.pro_partial_on_off_output_tuples,
    rule=res_timevar_output_minfraction_rampup_rule,
    doc='Output may not increase faster than the minimal working capacity')
```

```
def res_timevar_output_minfraction_rampup_rule(m, tm, stf, sit, pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                m.process_dict['min-fraction'][(stf, sit, pro)] *
                m.r_out_dict[(stf, pro, com)] *
                m.eff_factor_dict[(sit, pro)][stf, tm] >=
                m.e_pro_out[tm, stf, sit, pro, com])
```

(continues on next page)

(continued from previous page)

```

else:
    return pyomo.Constraint.Skip

```

If the process has both partial operation and time variable efficiency, the code changes to:

```

m.res_partial_timevar_output_minfraction_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_divides_minfraction_output_tuples &
        m.pro_partial_on_off_output_tuples & m.pro_timevar_output_tuples,
    rule=res_partial_timevar_output_minfraction_rampup_rule,
    doc='Output may not increase faster than the minimal working capacity')

```

```

def res_partial_timevar_output_minfraction_rampup_rule(m, tm, stf, sit,
    pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
            m.cap_pro[stf, sit, pro] * m.dt *
            m.process_dict['min-fraction'][(stf, sit, pro)] *
            m.r_out_min_fraction_dict[(stf, pro, com)] *
            m.eff_factor_dict[(sit, pro)][stf, tm] >=
            m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip

```

Case II: The parameter process minimum load fraction \underline{P}_{yvp} is greater than the parameter process maximum power ramp up gradient $\overline{PG}_{yvp}^{\text{up}}$, but is not divisible with it. It is defined and calculated by the following code fragment:

```

m.res_output_minfraction_rampup_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_not_divides_minfraction_output_tuples -
        m.pro_partial_on_off_output_tuples - m.pro_timevar_output_tuples,
    rule=res_output_minfraction_rampup_rampup_rule,
    doc='Output may not increase faster than the first multiple of the'
        'ramping up gradient greater than the minimal working capacity')

```

```

def res_output_minfraction_rampup_rampup_rule(m, tm, stf, sit, pro, com):
    ramp_up = m.process_dict['ramp-up-grad'][(stf, sit, pro)]
    min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]

    first_output_value = (math.floor(min_fraction / ramp_up) + 1) * ramp_up
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
            m.cap_pro[stf, sit, pro] * m.dt *
            first_output_value *
            m.r_out_dict[(stf, pro, com)] >=
            m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip

```

If the process has partial operation, the code changes to:

```

m.res_partial_output_minfraction_rampup_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_not_divides_minfraction_output_tuples &
        m.pro_partial_on_off_output_tuples - m.pro_timevar_output_tuples,
    rule=res_partial_output_minfraction_rampup_rampup_rule,

```

(continues on next page)

(continued from previous page)

```
doc='Output may not increase faster than the first multiple of the'
    'ramping up gradient greater than the minimal working capacity')
```

```
def res_partial_output_minfraction_rampup_rampup_rule(m, tm, stf, sit, pro,
    ↪ com):
    ramp_up = m.process_dict['ramp-up-grad'][(stf, sit, pro)]
    min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]

    first_output_value = (math.floor(min_fraction / ramp_up) + 1) * ramp_up
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                first_output_value *
                m.r_out_min_fraction_dict[(stf, pro, com)] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip
```

If the process has time variable efficiency, the code changes to:

```
m.res_timevar_output_minfraction_rampup_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_not_divides_minfraction_output_tuples &
        m.pro_timevar_output_tuples - m.pro_partial_on_off_output_tuples,
    rule=res_timevar_output_minfraction_rampup_rampup_rule,
    doc='Output may not increase faster than the first multiple of the'
        'ramping up gradient greater than the minimal working capacity')
```

```
def res_timevar_output_minfraction_rampup_rampup_rule(m, tm, stf, sit, pro,
    ↪ com):
    ramp_up = m.process_dict['ramp-up-grad'][(stf, sit, pro)]
    min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]

    first_output_value = (math.floor(min_fraction / ramp_up) + 1) * ramp_up
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                first_output_value *
                m.r_out_dict[(stf, pro, com)] *
                m.eff_factor_dict[(sit, pro)][stf, tm] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip
```

If the process has both partial operation and time variable efficiency, the code changes to:

```
m.res_partial_timevar_output_minfraction_rampup_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_not_divides_minfraction_output_tuples &
        m.pro_partial_on_off_output_tuples & m.pro_timevar_output_tuples,
    rule=res_partial_timevar_output_minfraction_rampup_rampup_rule,
    doc='Output may not increase faster than the first multiple of the'
        'ramping up gradient greater than the minimal working capacity')
```

```
def res_partial_timevar_output_minfraction_rampup_rampup_rule(m, tm, stf,
    ↪ sit, pro, com):
```

(continues on next page)

(continued from previous page)

```

ramp_up = m.process_dict['ramp-up-grad'][(stf, sit, pro)]
min_fraction = m.process_dict['min-fraction'][(stf, sit, pro)]

first_output_value = (math.floor(min_fraction / ramp_up) + 1) * ramp_up
if tm != m.timesteps[1]:
    return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
            m.cap_pro[stf, sit, pro] * m.dt *
            first_output_value *
            m.r_out_min_fraction_dict[(stf, pro, com)] *
            m.eff_factor_dict[(sit, pro)][stf, tm] >=
            m.e_pro_out[tm, stf, sit, pro, com])
else:
    return pyomo.Constraint.Skip

```

Case III: The parameter process minimum load fraction \underline{P}_{yvp} is smaller than the parameter process maximum power ramp up gradient $\overline{PG}_{yvp}^{\text{up}}$. It is defined and calculated by the following code fragment:

```

m.res_output_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_bigger_minfraction_output_tuples -
        m.pro_partial_on_off_output_tuples - m.pro_timevar_output_tuples,
    rule=res_output_rampup_rule,
    doc='Output may not increase faster than the ramping up gradient')

```

```

def res_output_rampup_rule(m, tm, stf, sit, pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                m.process_dict['ramp-up-grad'][(stf, sit, pro)] *
                m.r_out_dict[(stf, pro, com)] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip

```

If the process has partial operation, the code changes to:

```

m.res_partial_output_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_bigger_minfraction_output_tuples &
        m.pro_partial_on_off_output_tuples - m.pro_timevar_output_tuples,
    rule=res_partial_output_rampup_rule,
    doc='Output may not increase faster than the ramping up gradient')

```

```

def res_partial_output_rampup_rule(m, tm, stf, sit, pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                m.process_dict['ramp-up-grad'][(stf, sit, pro)] *
                m.r_out_min_fraction_dict[(stf, pro, com)] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip

```

If the process has time variable efficiency, the code changes to:

```

m.res_timevar_output_rampup = pyomo.Constraint(

```

(continues on next page)

(continued from previous page)

```
m.tm, m.pro_rampup_bigger_minfraction_output_tuples &
    m.pro_timevar_output_tuples - m.pro_partial_on_off_output_tuples,
rule=res_timevar_output_rampup_rule,
doc='Output may not increase faster than the ramping up gradient')
```

```
def res_timevar_output_rampup_rule(m, tm, stf, sit, pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                m.process_dict['ramp-up-grad'][(stf, sit, pro)] *
                m.r_out_dict[(stf, pro, com)] *
                m.eff_factor_dict[(sit, pro)][stf, tm] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip
```

If the process has both partial operation and time variable efficiency, the code changes to:

```
m.res_partial_timevar_output_rampup = pyomo.Constraint(
    m.tm, m.pro_rampup_bigger_minfraction_output_tuples &
        m.pro_partial_on_off_output_tuples & m.pro_timevar_output_tuples,
    rule=res_partial_timevar_output_rampup_rule,
    doc='Output may not increase faster than the ramping up gradient')
```

```
def res_partial_timevar_output_rampup_rule(m, tm, stf, sit, pro, com):
    if tm != m.timesteps[1]:
        return (m.e_pro_out[tm - 1, stf, sit, pro, com] +
                m.cap_pro[stf, sit, pro] * m.dt *
                m.process_dict['ramp-up-grad'][(stf, sit, pro)] *
                m.r_out_min_fraction_dict[(stf, pro, com)] *
                m.eff_factor_dict[(sit, pro)][stf, tm] >=
                m.e_pro_out[tm, stf, sit, pro, com])
    else:
        return pyomo.Constraint.Skip
```

Process Start-Up Rule: The constraint process start-up rule marks in the variable process start marker σ_{yvpt} whether a process p started in timestep t or not. The mathematical explanation of this rule is given in *Advanced Processes*.

In script `AdvancedProcesses.py` the constraint process start ups rule is defined and calculated by the following code fragment:

```
m.res_start_up = pyomo.Constraint(
    m.tm, m.pro_start_up_tuples,
    rule=res_start_ups_rule,
    doc='start >= on_off(t) - on_off(t-1)')
```

```
def res_start_up_rule(m, t, stf, sit, pro):
    return (m.start_up[t, stf, sit, pro] >= m.on_off[t, stf, sit, pro] -
            m.on_off[t - 1, stf, sit,
↪pro])
```

Transmission Constraints

Transmission Capacity Rule: The constraint transmission capacity rule defines the variable total transmission capacity κ_{yaf} . The variable total transmission capacity is defined by the constraint as the sum of the variable transmission capacity installed K_{yaf} and the variable new transmission capacity $\hat{\kappa}_{yaf}$. The mathematical explanation of this rule is given in *Multinode optimization model*.

In script `transmission.py` the constraint transmission capacity rule is defined and calculated by the following code fragment:

```
m.def_transmission_capacity = pyomo.Constraint(
    m.tra_tuples,
    rule=def_transmission_capacity_rule,
    doc='total transmission capacity = inst-cap + new capacity')

def def_transmission_capacity_rule(m, stf, sin, sout, tra, com):
    if m.mode['int']:
        if (sin, sout, tra, com, stf) in m.inst_tra_tuples:
            if (min(m.stf), sin, sout, tra, com) in m.tra_const_cap_dict:
                cap_tra = m.transmission_dict['inst-cap'][
                    (min(m.stf), sin, sout, tra, com)]
            else:
                cap_tra = (
                    sum(m.cap_tra_new[stf_built, sin, sout, tra, com]
                        for stf_built in m.stf
                        if (sin, sout, tra, com, stf_built, stf) in
                            m.operational_tra_tuples) +
                    m.transmission_dict['inst-cap']
                        [(min(m.stf), sin, sout, tra, com)])
        else:
            cap_tra = (
                sum(m.cap_tra_new[stf_built, sin, sout, tra, com]
                    for stf_built in m.stf
                    if (sin, sout, tra, com, stf_built, stf) in
                        m.operational_tra_tuples))
    else:
        if (stf, sin, sout, tra, com) in m.tra_const_cap_dict:
            cap_tra = \
                m.transmission_dict['inst-cap'][(stf, sin, sout, tra, com)]
        else:
            cap_tra = (m.cap_tra_new[stf, sin, sout, tra, com] +
                m.transmission_dict['inst-cap'][
                    (stf, sin, sout, tra, com)])

    return cap_tra
```

Transmission New Capacity Rule: The constraint transmission new capacity rule defines the variable new transmission capacity $\hat{\kappa}_{yaf}$. This variable is defined by the constraint as the product of the parameter transmission new capacity block K_{yaf}^{block} and the variable new transmission capacity units β_{yaf} . The mathematical explanation of this rule is given in *Multinode optimization model*.

In script `transmission.py` the constraint transmission output rule is defined and calculated by the following code fragment:

```
m.def_cap_tra_new = pyomo.Constraint(
    m.tra_block_tuples,
```

(continues on next page)

(continued from previous page)

```
rule=def_cap_tra_new_rule,
doc='cap_tra_new = tra_block * cap_tra_new')
```

```
def def_cap_tra_new_rule(m, stf, sin, sout, tra, com):
    return (m.cap_tra_new[stf, sin, sout, tra, com] ==
            m.tra_cap_unit[stf, sin, sout, tra, com] *
            m.transmission_dict['tra_block'][(stf, sin, sout, tra, com)])
```

Transmission Output Rule: The constraint transmission output rule defines the variable transmission output commodity flow π_{yaf}^{out} . The variable transmission output commodity flow is defined by the constraint as the product of the variable transmission input commodity flow π_{yaf}^{in} and the parameter transmission efficiency e_{yaf} . The mathematical explanation of this rule is given in [Multinode optimization model](#).

In script `transmission.py` the constraint transmission output rule is defined and calculated by the following code fragment:

```
m.def_transmission_output = pyomo.Constraint(
    m.tm, m.tra_tuples,
    rule=def_transmission_output_rule,
    doc='transmission output = transmission input * efficiency')
```

```
def def_transmission_output_rule(m, tm, stf, sin, sout, tra, com):
    return (m.e_tra_out[tm, stf, sin, sout, tra, com] ==
            m.e_tra_in[tm, stf, sin, sout, tra, com] *
            m.transmission_dict['eff'][(stf, sin, sout, tra, com)])
```

Transmission Input By Capacity Rule: The constraint transmission input by capacity rule limits the variable transmission input commodity flow π_{yaf}^{in} . This constraint prevents the transmission power from exceeding the possible power input capacity of the line. The constraint states that the variable transmission input commodity flow π_{yaf}^{in} must be less than or equal to the variable total transmission capacity κ_{yaf} , scaled by the size of the time steps :math: \Delta t. The mathematical explanation of this rule is given in [Multinode optimization model](#).

In script `transmission.py` the constraint transmission input by capacity rule is defined and calculated by the following code fragment:

```
m.res_transmission_input_by_capacity = pyomo.Constraint(
    m.tm, m.tra_tuples,
    rule=res_transmission_input_by_capacity_rule,
    doc='transmission input <= total transmission capacity')
```

```
def res_transmission_input_by_capacity_rule(m, tm, stf, sin, sout, tra,
    com):
    return (m.e_tra_in[tm, stf, sin, sout, tra, com] <=
            m.dt * m.cap_tra[stf, sin, sout, tra, com])
```

Transmission Capacity Limit Rule: The constraint transmission capacity limit rule limits the variable total transmission capacity κ_{yaf} . This constraint restricts a transmission f through an arc a in support timeframe y from having more total power output capacity than an upper bound and having less than a lower bound. The constraint states that the variable total transmission capacity κ_{yaf} must be greater than or equal to the parameter transmission capacity lower bound \underline{K}_{yaf} and less than or equal to the parameter transmission capacity upper bound \overline{K}_{yaf} . The mathematical explanation of this rule is given

in *Multinode optimization model*.

In script `transmission.py` the constraint transmission capacity limit rule is defined and calculated by the following code fragment:

```
m.res_transmission_capacity = pyomo.Constraint(
    m.tra_tuples,
    rule=res_transmission_capacity_rule,
    doc='transmission.cap-lo <= total transmission capacity <= '
        'transmission.cap-up')

def res_transmission_capacity_rule(m, stf, sin, sout, tra, com):
    return (m.transmission_dict['cap-lo'][(stf, sin, sout, tra, com)],
            m.cap_tra[stf, sin, sout, tra, com],
            m.transmission_dict['cap-up'][(stf, sin, sout, tra, com)])
```

Transmission Symmetry Rule: The constraint transmission symmetry rule defines the power capacities of incoming and outgoing arcs a, a' of a transmission f in support timeframe y . The constraint states that the power capacities κ_{af} of the incoming arc a and the complementary outgoing arc a' between two sites must be equal. The mathematical explanation of this rule is given in *Multinode optimization model*.

In script `transmission.py` the constraint transmission symmetry rule is defined and calculated by the following code fragment:

```
m.res_transmission_symmetry = pyomo.Constraint(
    m.tra_tuples,
    rule=res_transmission_symmetry_rule,
    doc='total transmission capacity must be symmetric in both directions')

def res_transmission_symmetry_rule(m, stf, sin, sout, tra, com):
    return m.cap_tra[stf, sin, sout, tra, com] == (m.cap_tra
                                                    [stf, sout, sin, tra,
                                                    ↪com])
```

DCPF Transmission Constraints

The following constraints are included in the model if the optional DC Power Flow feature is activated.

DC Power Flow Rule: The constraint DC Power Flow rule defines the power flow of transmission lines, which are modelled with DCPF. This constraint states that the power flow on a transmission line is equal to the product of voltage angle differences of two connecting sites v_{out} and v_{in} and the admittance of the transmission line. This constraint is only applied to the transmission lines modelled with DCPF. The mathematical explanation of this rule is given in *Multinode optimization model*. In script `transmission.py` the constraint DC Power Flow Rule is defined and calculated by the following code fragment:

```
m.def_dc_power_flow = pyomo.Constraint(
    m.tm, m.tra_tuples_dc,
    rule=def_dc_power_flow_rule,
    doc='transmission output = (angle(in)-angle(out)) / 57.2958 '
        '* -1 * (-1/reactance) * (base voltage)^2')
```

```
def def_dc_power_flow_rule(m, tm, stf, sin, sout, tra, com):
    return (m.e_tra_in[tm, stf, sin, sout, tra, com] ==
            (m.voltage_angle[tm, stf, sin] - m.voltage_angle[tm, stf,
→sout]) / 57.2958 * -1 *
            (-1 / m.transmission_dict['reactance'][(stf, sin, sout, tra,
→com)]))
            * m.site_dict['base-voltage'][(stf, sin)]**2)
```

DCPF Transmission Input By Capacity Rule: The constraint DCPF transmission input by capacity rule expands the constraint transmission input by capacity rule for transmission lines modelled with DCPF. This constraint limits the variable transmission input commodity flow π_{yaf}^{in} of DCPF transmission lines also with a lower bound. This constraint prevents the absolute value of the transmission power from exceeding the possible power input capacity of the line especially when the transmission power can be negative. The constraint states that the additive inverse of variable transmission input commodity flow $-\pi_{yaf}^{\text{in}}$ must be less than or equal to the variable total transmission capacity κ_{yaf} , scaled by the size of the time steps :math: \Delta t. This constraint is only applied to the transmission lines modelled with DCPF. The mathematical explanation of this rule is given in [Multinode optimization model](#).

In script `transmission.py` the constraint transmission input by capacity rule is defined and calculated by the following code fragment:

```
m.res_transmission_dc_input_by_capacity = pyomo.Constraint(
    m.tm, m.tra_tuples_dc,
    rule=res_transmission_dc_input_by_capacity_rule,
    doc='-dcpf transmission input <= total transmission capacity')
```

Voltage Angle Limit Rule: The constraint voltage angle limit rule limits the maximum and minimum difference of voltage angles θ_{yvt} of two sites v_{out} and v_{in} connected with a DCPF transmission line with the parameter voltage angle difference limit \overline{dl}_{yaf} . This constraint is only applied to the transmission lines modelled with DCPF. The mathematical explanation of this rule is given in [Multinode optimization model](#). In script `transmission.py` the constraint voltage angle limit rule is defined and given by the following code fragment:

```
m.def_angle_limit = pyomo.Constraint(
    m.tm, m.tra_tuples_dc,
    rule=def_angle_limit_rule,
    doc='-angle limit < angle(in) - angle(out) < angle limit')
```

```
def def_angle_limit_rule(m, tm, stf, sin, sout, tra, com):
    return (- m.transmission_dict['difflimit'][(stf, sin, sout, tra, com)],
            (m.voltage_angle[tm, stf, sin] - m.voltage_angle[tm, stf,
→sout])),
            m.transmission_dict['difflimit'][(stf, sin, sout, tra, com)])
```

Absolute Transmission Flow Constraints: The two absolute transmission flow constraints are included in the model to create the variable absolute value of transmission commodity flow π_{yaf}^{in} . By limiting the negative $-\pi_{yaf}^{\text{in}}$ and positive π_{yaf}^{in} of substitute variable “e_tra_abs” with the variable π_{yaf}^{in} and minimizing the substitute value π_{yaf}^{in} the absolute value of transmission commodity flow is retrieved. These constraints are only applied to the transmission lines modelled with DCPF. The mathematical explanation of these rules are given in [Multinode optimization model](#). In script `transmission.py` the constraint Absolute Transmission Flow Constraints are defined and given by the following code fragment:

```
m.e_tra_abs1 = pyomo.Constraint(
    m.tm, m.tra_tuples_dc,
    rule=e_tra_abs_rule1,
    doc='transmission dc input <= absolute transmission dc input')
m.e_tra_abs2 = pyomo.Constraint(
    m.tm, m.tra_tuples_dc,
    rule=e_tra_abs_rule2,
    doc='-transmission dc input <= absolute transmission dc input')
```

```
def e_tra_abs_rule1(m, tm, stf, sin, sout, tra, com):
    return (m.e_tra_in[tm, stf, sin, sout, tra, com] <=
            m.e_tra_abs[tm, stf, sin, sout, tra, com])
```

```
def e_tra_abs_rule2(m, tm, stf, sin, sout, tra, com):
    return (-m.e_tra_in[tm, stf, sin, sout, tra, com] <=
            m.e_tra_abs[tm, stf, sin, sout, tra, com])
```

Transmission Symmetry Rule: The above mentioned constraint transmission symmetry rule is only applied to the transmission lines modelled with transport model if the DCPF is activated. Since the DCPF transmission lines do not include the complementary arcs, this constraint is ignored for these transmission lines. For this reason, the constraint is indexed with the transmission tuple set `m.tra_tuples_tp` if the DCPF is activated.

In script `transmission.py` the constraint transmission symmetry rule is defined as following if the DCPF is activated:

```
m.res_transmission_symmetry = pyomo.Constraint(
    m.tra_tuples_tp,
    rule=res_transmission_symmetry_rule,
    doc='total transmission capacity must be symmetric in both directions')
```

Storage Constraints

Storage State Rule: The constraint storage state rule is the main storage constraint and it defines the storage energy content of a storage s in a site v in support timeframe y at a timestep t . This constraint calculates the storage energy content at a timestep t by adding or subtracting differences, such as ingoing and outgoing energy, to/from a storage energy content at a previous timestep $t - 1$ multiplied by 1 minus the self-discharge rate d_{yvs} (which is scaled exponentially with the timestep size δt). Here ingoing energy is given by the product of the variable storage input commodity flow $\epsilon_{yvs}^{\text{in}}$ and the parameter storage efficiency during charge e_{yvs}^{in} . Outgoing energy is given by the variable storage output commodity flow $\epsilon_{yvs}^{\text{out}}$ divided by the parameter storage efficiency during discharge e_{yvs}^{out} . The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage state rule is defined and calculated by the following code fragment:

```
m.def_storage_state = pyomo.Constraint(
    m.tm, m.sto_tuples,
    rule=def_storage_state_rule,
    doc='storage[t] = (1 - selfdischarge) * storage[t-1] + input * eff_in -
    → output / eff_out')
```

```
def def_storage_state_rule(m, t, stf, sit, sto, com):
    return (m.e_sto_con[t, stf, sit, sto, com] ==
            m.e_sto_con[t - 1, stf, sit, sto, com] *
            (1 - m.storage_dict['discharge']
             [(stf, sit, sto, com)]) ** m.dt.value +
            m.e_sto_in[t, stf, sit, sto, com] *
            m.storage_dict['eff-in'][(stf, sit, sto, com)] -
            m.e_sto_out[t, stf, sit, sto, com] /
            m.storage_dict['eff-out'][(stf, sit, sto, com)])
```

Storage Power Rule: The constraint storage power rule defines the variable total storage power κ_{yvs}^p . The variable total storage power is defined by the constraint as the sum of the parameter storage power installed K_{yvs}^p and the variable new storage power $\hat{\kappa}_{yvs}^p$. The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage power rule is defined and calculated by the following code fragment:

```
m.def_storage_power = pyomo.Constraint(
    m.sto_tuples,
    rule=def_storage_power_rule,
    doc='storage power = inst-cap + new power')
```

```
def def_storage_power_rule(m, stf, sit, sto, com):
    if m.mode['int']:
        if (sit, sto, com, stf) in m.inst_sto_tuples:
            if (min(m.stf), sit, sto, com) in m.sto_const_cap_p_dict:
                cap_sto_p = m.storage_dict['inst-cap-p'][(min(m.stf), sit, sto, com)]
            else:
                cap_sto_p = (
                    sum(m.cap_sto_p_new[stf_built, sit, sto, com]
                       for stf_built in m.stf
                       if (sit, sto, com, stf_built, stf) in
                           m.operational_sto_tuples) +
                    m.storage_dict['inst-cap-p'][(min(m.stf), sit, sto, com)])
        else:
            cap_sto_p = (
                sum(m.cap_sto_p_new[stf_built, sit, sto, com]
                   for stf_built in m.stf
                   if (sit, sto, com, stf_built, stf) in
                       m.operational_sto_tuples))
    else:
        if (stf, sit, sto, com) in m.sto_const_cap_p_dict:
            cap_sto_p = m.storage_dict['inst-cap-p'][(stf, sit, sto, com)]
        else:
            cap_sto_p = (m.cap_sto_p_new[stf, sit, sto, com] +
                         m.storage_dict['inst-cap-p'][(stf, sit, sto, com)])

    return cap_sto_p
```

Storage Capacity Rule: The constraint storage capacity rule defines the variable total storage size κ_{yvs}^c . The variable total storage size is defined by the constraint as the sum of the parameter storage content installed K_{yvs}^c and the variable new storage size $\hat{\kappa}_{yvs}^c$. The mathematical explanation of this rule is given

in *Energy Storage*.

In script `storage.py` the constraint storage capacity rule is defined and calculated by the following code fragment:

```
m.def_storage_capacity = pyomo.Constraint(
    m.sto_tuples,
    rule=def_storage_capacity_rule,
    doc='storage capacity = inst-cap + new capacity')
```

```
def def_storage_capacity_rule(m, stf, sit, sto, com):
    if m.mode['int']:
        if (sit, sto, com, stf) in m.inst_sto_tuples:
            if (min(m.stf), sit, sto, com) in m.sto_const_cap_c_dict:
                cap_sto_c = m.storage_dict['inst-cap-c'][(min(m.stf), sit, sto,
→com)]
            else:
                cap_sto_c = (
                    sum(m.cap_sto_c_new[stf_built, sit, sto, com]
                        for stf_built in m.stf
                        if (sit, sto, com, stf_built, stf) in
                            m.operational_sto_tuples) +
                    m.storage_dict['inst-cap-c'][(min(m.stf), sit, sto,
→com)])
        else:
            cap_sto_c = (
                sum(m.cap_sto_c_new[stf_built, sit, sto, com]
                    for stf_built in m.stf
                    if (sit, sto, com, stf_built, stf) in
                        m.operational_sto_tuples))
        else:
            if (stf, sit, sto, com) in m.sto_const_cap_c_dict:
                cap_sto_c = m.storage_dict['inst-cap-c'][(stf, sit, sto, com)]
            else:
                cap_sto_c = (m.cap_sto_c_new[stf, sit, sto, com] +
                    m.storage_dict['inst-cap-c'][(stf, sit, sto,
→com)])

    return cap_sto_c
```

Storage New Capacity Rule: The constraint storage new capacity rule defines the newly installed capacity of a storage \hat{K}_{yvs}^c . This variable is defined by the constraint as the product of the variable new storage size units β_{yvs}^c and the parameter storage new capacity block $K_{yvs}^{c,block}$. The mathematical explanation of this rule is given in *Energy Storage*.

In script `storage.py` the constraint storage capacity rule is defined and calculated by the following code fragment:

```
m.def_new_cap_sto_c = pyomo.Constraint(
    m.sto_block_c_tuples,
    rule=def_new_cap_sto_c_rule,
    doc='cap_sto_c_new = cap_sto_c_unit * c-block')
```

```
def def_new_cap_sto_c_rule(m, stf, sit, sto, com):
    return (m.cap_sto_c_new[stf, sit, sto, com] ==
        m.sto_cap_c_unit[stf, sit, sto, com] *
        m.sto_block_c_dict[stf, sit, sto, com])
```

Storage New Power Rule: The constraint storage new power rule defines the newly installed power of a storage $\hat{\kappa}_{yvs}^p$. This variable is defined by the constraint as the product of the variable new power size units β_{yvs}^p and the parameter storage new power block $K_{yvs}^{p,block}$. The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage capacity rule is defined and calculated by the following code fragment:

```
m.def_new_cap_sto_p = pyomo.Constraint(
    m.sto_block_p_tuples,
    rule=def_new_cap_sto_p_rule,
    doc='cap_sto_p_new = cap_sto_p_unit * p-block')
```

```
def def_new_cap_sto_p_rule(m, stf, sit, sto, com):
    return (m.cap_sto_p_new[stf, sit, sto, com] ==
            m.sto_cap_p_unit[stf, sit, sto, com] *
            m.sto_block_p_dict[stf, sit, sto, com])
```

Storage Input By Power Rule: The constraint storage input by power rule limits the variable storage input commodity flow ϵ_{yvs}^{in} . This constraint restricts a storage s in a site v and support timeframe y at a timestep t from having more input power than the storage power capacity. The constraint states that the variable ϵ_{yvs}^{in} must be less than or equal to the variable total storage power κ_{yvs}^p , scaled by the size of the time steps Δt . The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage input by power rule is defined and calculated by the following code fragment:

```
m.res_storage_input_by_power = pyomo.Constraint(
    m.tm, m.sto_tuples,
    rule=res_storage_input_by_power_rule,
    doc='storage input <= storage power')
```

```
def res_storage_input_by_power_rule(m, t, stf, sit, sto, com):
    return (m.e_sto_in[t, stf, sit, sto, com] <= m.dt *
            m.cap_sto_p[stf, sit, sto, com])
```

Storage Output By Power Rule: The constraint storage output by power rule limits the variable storage output commodity flow ϵ_{vst}^{out} . This constraint restricts a storage s in a site v and support timeframe y at a timestep t from having more output power than the storage power capacity. The constraint states that the variable ϵ_{vst}^{out} must be less than or equal to the variable total storage power κ_{yvs}^p , scaled by the size of the time steps Δt . The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage output by power rule is defined and calculated by the following code fragment:

```
m.res_storage_output_by_power = pyomo.Constraint(
    m.tm, m.sto_tuples,
    rule=res_storage_output_by_power_rule,
    doc='storage output <= storage power')
```

```
def res_storage_output_by_power_rule(m, t, stf, sit, sto, co):
    return (m.e_sto_out[t, stf, sit, sto, co] <= m.dt *
            m.cap_sto_p[stf, sit, sto, co])
```

Storage State By Capacity Rule: The constraint storage state by capacity rule limits the variable storage

energy content $\epsilon_{yvs}^{\text{con}}$. This constraint restricts a storage s in a site v and support timeframe y at a timestep t from having more storage content than the storage content capacity. The constraint states that the variable $\epsilon_{yvs}^{\text{con}}$ must be less than or equal to the variable total storage size κ_{yvs}^{c} . The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage state by capacity rule is defined and calculated by the following code fragment.

```
m.res_storage_state_by_capacity = pyomo.Constraint(
    m.t, m.sto_tuples,
    rule=res_storage_state_by_capacity_rule,
    doc='storage content <= storage capacity')
```

```
def res_storage_state_by_capacity_rule(m, t, stf, sit, sto, com):
    return (m.e_sto_con[t, stf, sit, sto, com] <=
            m.cap_sto_c[stf, sit, sto, com])
```

Storage Power Limit Rule: The constraint storage power limit rule limits the variable total storage power κ_{yvs}^{p} . This constraint restricts a storage s in a site v and support timeframe y from having more total power output capacity than an upper bound and having less than a lower bound. The constraint states that the variable total storage power κ_{yvs}^{p} must be greater than or equal to the parameter storage power lower bound $\underline{K}_{yvs}^{\text{p}}$ and less than or equal to the parameter storage power upper bound $\overline{K}_{yvs}^{\text{p}}$. The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage power limit rule is defined and calculated by the following code fragment:

```
m.res_storage_power = pyomo.Constraint(
    m.sto_tuples,
    rule=res_storage_power_rule,
    doc='storage.cap-lo-p <= storage power <= storage.cap-up-p')
```

```
def res_storage_power_rule(m, stf, sit, sto, com):
    return (m.storage_dict['cap-lo-p'][(stf, sit, sto, com)],
            m.cap_sto_p[stf, sit, sto, com],
            m.storage_dict['cap-up-p'][(stf, sit, sto, com)])
```

Storage Capacity Limit Rule: The constraint storage capacity limit rule limits the variable total storage size κ_{yvs}^{c} . This constraint restricts a storage s in a site v and support timeframe y from having more total storage content capacity than an upper bound and having less than a lower bound. The constraint states that the variable total storage size κ_{yvs}^{c} must be greater than or equal to the parameter storage content lower bound $\underline{K}_{yvs}^{\text{c}}$ and less than or equal to the parameter storage content upper bound $\overline{K}_{yvs}^{\text{c}}$. The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage capacity limit rule is defined and calculated by the following code fragment:

```
m.res_storage_capacity = pyomo.Constraint(
    m.sto_tuples,
    rule=res_storage_capacity_rule,
    doc='storage.cap-lo-c <= storage capacity <= storage.cap-up-c')
```

```
def res_storage_capacity_rule(m, stf, sit, sto, com):
    return (m.storage_dict['cap-lo-c'][(stf, sit, sto, com)],
```

(continues on next page)

(continued from previous page)

```
m.cap_sto_c[stf, sit, sto, com],
m.storage_dict['cap-up-c'][(stf, sit, sto, com)])
```

Initial And Final Storage State Rule: The constraint initial and final storage state rule defines and restricts the variable storage energy content $\epsilon_{yvs}^{\text{con}}$ of a storage s in a site v and support timeframe y at the initial timestep t_1 and at the final timestep t_N . There are two distinct cases:

1. The initial and final storage states are specified by a value of the parameter I_{yvs} between 0 and 1. 2. I_{yvs} is not specified (e.g. by setting it '#NV' in the input sheet). In this case the initial and final storage state are still equal but variable.

In case 1 the constraints are written in the following way:

Initial storage state: Initial storage represents the storage state in a storage at the beginning of the simulation. The variable storage energy content $\epsilon_{yvs}^{\text{con}}$ at the initial timestep t_1 is defined by this constraint. The constraint states that the variable $\epsilon_{yvs}^{\text{con}}$ must be equal to the product of the parameters storage content installed K_{yvs}^c and initial and final state of charge I_{yvs} .

Final storage state: Final storage represents the storage state in a storage at the end of the simulation. The variable storage energy content $\epsilon_{yvs}^{\text{con}}$ at the final timestep t_N is restricted by this constraint. The constraint states that the variable $\epsilon_{yvs}^{\text{con}}$ must be greater than or equal to the product of the parameters storage content installed K_{yvs}^c and initial and final state of charge I_{yvs} . The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint initial and final storage state rule is then defined and calculated by the following code fragment:

```
m.res_initial_and_final_storage_state = pyomo.Constraint(
    m.t, m.sto_init_bound_tuples,
    rule=res_initial_and_final_storage_state_rule,
    doc='storage content initial == and final >= storage.init * capacity')
```

In case 2 the constraint becomes a lot easier, since the initial and final state are simply compared to each other by the following inequality:

$$\forall v \in V, s \in S: \epsilon_{vst_1}^{\text{con}} \leq \epsilon_{vst_N}^{\text{con}}$$

In script `storage.py` the constraint initial and final storage state rule is then defined and calculated by the following code fragment:

```
m.res_initial_and_final_storage_state_var = pyomo.Constraint(
    m.t, m.sto_tuples - m.sto_init_bound_tuples,
    rule=res_initial_and_final_storage_state_var_rule,
    doc='storage content initial <= final, both variable')
```

Storage Energy to Power Ratio Rule: For certain type of storage technologies, the power and energy capacities cannot be independently sized but are dependent to each other. Hence, the constraint storage energy to power ratio rule sets a linear dependence between the capacities through a user-defined “energy to power ratio” $k_{yvs}^{\text{E/P}}$. It has to be noted that this constraint is only active for the storages with a positive value under the column “ep-ratio” in the input file, and when this value is not given, the power and energy capacities can be sized independently. The mathematical explanation of this rule is given in [Energy Storage](#).

In script `storage.py` the constraint storage energy to power rule is then defined and calculated by the following code fragment:

```
m.def_storage_energy_power_ratio = pyomo.Constraint(
    m.sto_en_to_pow_tuples,
    rule=def_storage_energy_power_ratio_rule,
    doc='storage capacity = storage power * storage E2P ratio')
```

```
def def_storage_energy_power_ratio_rule(m, stf, sit, sto, com):
    return (m.cap_sto_c[stf, sit, sto, com] == m.cap_sto_p[stf, sit, sto,
→com] *
            m.storage_dict['ep-ratio'][(stf, sit, sto, com)])
```

Cost Constraints

The variable total system cost ζ is calculated by the cost function. In cases of CO₂-minimization the total system cost is constrained by the following expression:


$$\zeta = \zeta_{\text{inv}} + \zeta_{\text{fix}} + \zeta_{\text{var}} + \zeta_{\text{fuel}} + \zeta_{\text{rev}} + \zeta_{\text{pur}} + \zeta_{\text{startup}} + \zeta_{\text{env}} \leq \bar{I}_{\text{cost}}$$

This constraint is given in `model.py` by the following code fragment.

```
def res_global_cost_limit_rule(m, stf):
    if math.isinf(m.global_prop_dict["value"][stf, "Cost limit"]):
        return pyomo.Constraint.Skip
    elif m.global_prop_dict["value"][stf, "Cost limit"] >= 0:
        return (pyomo.summation(m.costs) <= m.global_prop_dict["value"]
                [stf, "Cost limit"])
    else:
        return pyomo.Constraint.Skip
```

1.3.2 ‘urbs’ module description

This part gives a brief overview over the architecture of the program. The data flow in an urbs model is visualized in the following graph:

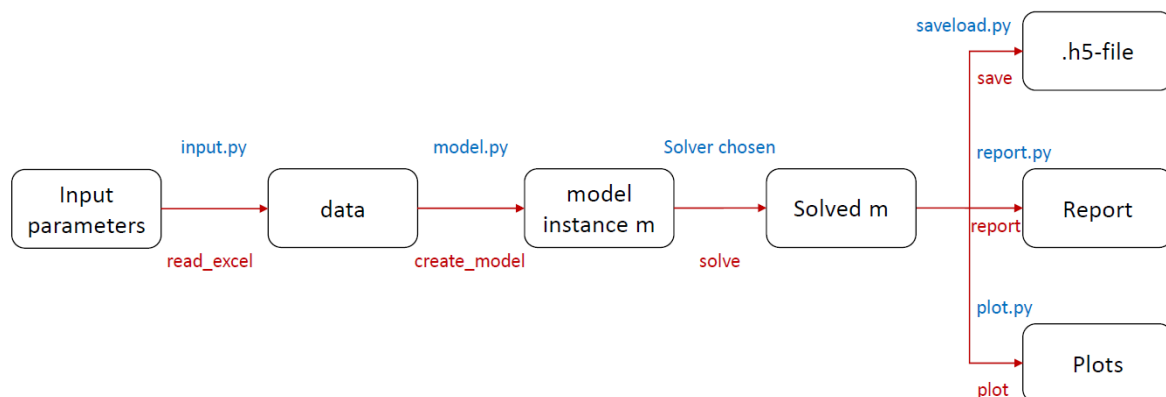

‘urbs’ uses a modular structure to build and execute the optimization and to automatically generate the results. All scripts are placed in the folder ‘urbs’. In subfolder ‘features’ constraint expressions for the mathematical model are defined. These will not be discussed here and only the highest level functions will be discussed. The scripts used for these are the following (in alphabetical order):

identify.py

In this scripts the dictionary of input dataframes 'data' is parsed to conclude the structure of the problem to be built.

input.py

This file handles the input and prepares the mathematical model itself.

model.py

This file just includes the central function used for model generation.

output.py

This file contains lower level functions to retrieve data from a solved model instance.

plot.py

This script generates automated output pictures using the function

report.py

This script handles the automated generation of an excel data sheet from the solved model instance.

runfunctions.py

This file contains the central function for running a predefined set of inputs or a scenario thereof.

saveload.py

This file contains two functions to save and load a collection of inputs and the corresponding outputs of a model instance.

scenarios.py

In this script scenario functions are defined. These are used to automatically change the inputs as given in dictionary 'data'. In this way multiple runs of similar model instances can be automated.

validation.py

This file makes sure that the input given is not leading to an infeasible or non-sensical model. It generates error messages for certain known errors. It is a organically growing script.

1.4 CoTraDis module

Continue here for the usage instructions on the coupled transmission-distribution system (CoTraDis) module.

1.4.1 Coupling of Transmission and Distribution System Modules

Overview

To completely understand the following new CoTraDis documentation you should already be familiar with the general urbs model (consult *Users guide* of the urbs framework). Before applying the developed CoTraDis model framework you should start with this overview that explains the underlying ideas of coupling transmission and distribution systems as developed in the master thesis of Beneharo Reveron Baecker: “Implementation of a novel energy system model coupling approach to co-optimize transmission and active distribution systems”, 2021. The related documentation is structured into four main parts:

1. The development of a model framework that enables the consideration of distribution systems. The implementations to consider their characteristics properly are described in *Distribution System Framework*.
2. An automated coupling of transmission and distribution system data. The implementation can be seen in the section *Automated Coupling*.
3. A suitable approach to reduce the computational complexity. The implementations make use of the typeperiod idea in combination with time series aggregation methods. It is described in detail in the section *Time Series Aggregation with Typeperiods*. If you want to understand the mathematical background of tsam, you should first have a look at the documentation of the open source *python tsam package* described by Kotzuer et al.
4. Finally the ‘*CoTraDis*’ *application guide* gives ideas on how to use the provided framework for future projects.

Distribution System Framework

This section explains the implementations to consider specific distribution system characteristics. Major additions & modifications were applied to the the following scripts:

- `model.py`:
- `transmission.py`:


which will be described below. | Before dealing with the code, a short summary of required aspects to consider will be given.

Distribution systems are different from transmission systems in a number of facets. Differences to highlight are the reactance-to-resistance ratio (X/R) and their common radial composition. Depending on these attributes an AC optimal-power-flow model may be helpful to deal with distribution system reactive power and voltage constraints. Hence, the “LinDistFlow” model linearization has been introduced into the given framework as shown in `transmission.py`. Besides, we enhanced the *urbs* framework by integrating several aspects that characterize classic distribution systems:

- radially-operated open ring grid segments

- a transformer between both system levels modelled with a boundary bus
- reactive power demand for households
- reactive power line flows and an apparent power line flow constraint
- a central reactive power compensation system
- inverters with a predefined permissible ratio of reactive to active power generation.

The microgrids to describe the distribution system can be freely defined with the microgrid input sheets. The predefined microgrid structure with their assigned technologies as provided in the input data are illustrated below:

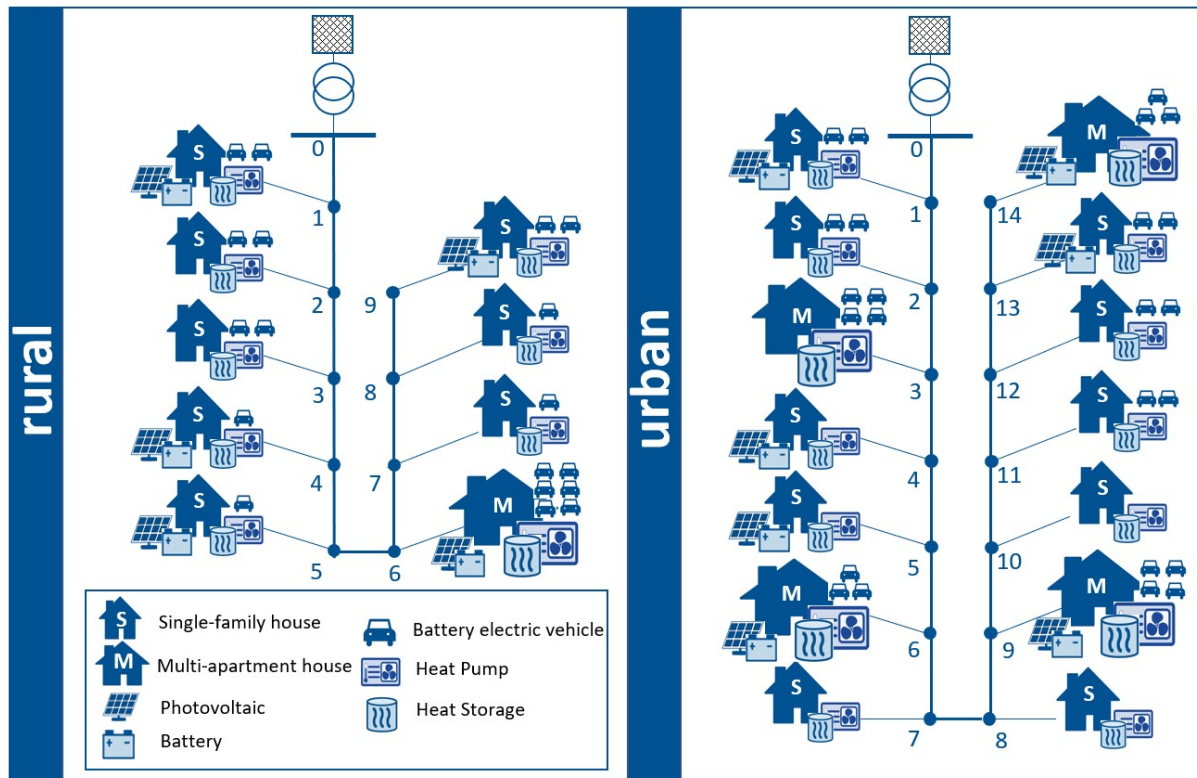

Implementations: model.py

The extensions within this module mainly include reactive power consideration for processes. In order to do so, all components located at distribution system nodes are identified with the ‘min-voltage’ parameter’ which is determined in the “sites” sheet of the microgrid input data. This set is used in this module and in the `urbs/transmission.py` module as explained later.

```
m.sit_tuples_ac = pyomo.Set(
    within=m.stf * m.sit,
    initialize=[(stf, site) for (stf, site) in m.sit_tuples
                if m.site_dict['min-voltage'][(stf, site)] > 0],
    doc='Combinations of support timeframes and sites with ac_
    ↳characteristics')
```

In this module the reactive power output share is typically indicated with the power factor ϕ that can be defined for each process in the input sheet. It describes the ratio of real power over apparent power. With this for instance PV-inverters can be enabled to provide inductive and capacitive reactive power. The

permissible ratio of active and reactive power output for generators is implemented into the model with the following rules that connect the reactive with the active power output by defining upper and lower generation limits for the previously defined set:

```
def def_process_output_reactive_rule1(m, tm, stf, sit, pro):
    return (m.e_pro_out[tm, stf, sit, pro, 'electricity-reactive'] <=
            m.e_pro_out[tm, stf, sit, pro, 'electricity']
            * math.tan(math.acos(m.process_dict['pf-min'][(stf, sit, pro)])))
def def_process_output_reactive_rule2(m, tm, stf, sit, pro):
    return (m.e_pro_out[tm, stf, sit, pro, 'electricity-reactive'] >=
            -m.e_pro_out[tm, stf, sit, pro, 'electricity']
            * math.tan(math.acos(m.process_dict['pf-min'][(stf, sit, pro)])))
```

Furthermore, a set with all boundary buses denoted as slackbuses representing the transformer on the distribution system site is defined as follows:

```
m.sit_slackbus = pyomo.Set(
    within=m.stf * m.sit,
    initialize=[(stf, site) for (stf, site) in m.sit_tuples
                if m.site_dict['ref-node'][(stf, site)] == 1],
    doc='Set of all reference nodes in defined microgrids')
```

In the `transmission.py` module this set is applied to define the voltage level of each microgrid as defined with the base-voltage parameters.

Implementations: `transmission.py`

Transmission lines can only transport one single commodity in the given model framework. Therefore, imaginary extra lines are created in the `transdisthelper.py` module. Active and reactive power flows are coupled with a redefined transmission line capacity constraint using a new rule that considers the apparent power:

```
def def_transmission_input_by_apparent_power_rule(m, tm, stf, sin, sout, tra, com):
    return (m.e_tra_in[tm, stf, sin, sout, tra, 'electricity']**2
            + m.e_tra_in[tm, stf, sin, sout, tra, 'electricity-reactive']**2
            <= (m.dt * m.cap_tra[stf, sin, sout, tra, com])**2)
```

To consider the correct lines in a coupled model the distribution system transmission tuple set is created for all predefined lines. The resistance is required in the input sheet to activate the distribution system linearization method. The resistance parameter should be greater than 0 and given in per-unit system. The new `m.def_ac_power_flow` constraint applies the following rule to the resulting tuple set of lines:

```
def def_ac_power_flow_rule(m, tm, stf, sin, sout, tra, com):
    return (m.voltage_squared[tm, stf, sin] == m.voltage_squared[tm, stf, sout] +
            2 * (m.transmission_dict['resistance'][(stf, sin, sout, tra, 'electricity')]
                * m.e_tra_in[tm, stf, sin, sout, tra, 'electricity']
                + m.transmission_dict['reactance'][(stf, sin, sout, tra, 'electricity-reactive')]
                * m.e_tra_in[tm, stf, sin, sout, tra, 'electricity-reactive']))
```

In comparison to the DC-OPF *Multinode optimization model* model, the key difference is that the nodal voltage magnitudes V^2 are related to the active and reactive power branch flows with the respective line impedance. After creating the new variable *voltage_squared* for this quantity

```
m.voltage_squared = pyomo.Var(
    m.tm, m.site_tuples_ac,
    within=pyomo.Reals,
    doc='Voltage^2 of a site')
```

another constraint is introduced in order to monitor the permissible voltage range for all distribution system sites included in a new set that has been defined in `urbs/model.py`. This is achieved with the new *def_voltage_limit* constraint applying the following rule:

```
def def_voltage_limit_rule(m, tm, stf, sin):
    return ((m.site_dict['base-voltage'][(stf, sin)] * m.site_dict[
        'min-voltage'][(stf, sin)])**2,
            m.voltage_squared[tm, stf, sin],
            (m.site_dict['base-voltage'][(stf, sin)] * m.site_dict['max-voltage']
             [(stf, sin)])**2)
```

Moreover, the voltage of all nodes within the introduced slackbus set is scaled to the base voltage of the respective grid, that is defined within the input sheet:

```
def def_slackbus_voltage_rule(m, tm, stf, sin):
    return (m.voltage_squared[tm, stf, sin] == m.site_dict['base-
        voltage'][(stf, sin)]**2)
```

Automated Coupling

A central goal in this work is to consider different system levels within a single multi-commodity energy system model for expansion and operation planning. A key aspect to realize this for our energy system planning approach is to integrate the bottom level microgrids within each associated top level region. In the following, a walkthrough on the `transdisthelper.py` script will be given to establish understanding regarding how the model coupling implementations work.

1. Import of Microgrid Data

Import microgrid data with a predefined selection list:

```
for set_number, set in enumerate(microgrid_set_list): # top region_
    microgrid_setting
    top_region_name = data['site'].index.get_level_values(1)[set_number]
    for type_nr, quantity_nr in enumerate(set):
        microgrid_entries = microgrid_data_initial[type_nr]['site'].index.
        get_level_values(1)
        n = 0
        while n < quantity_nr:
            microgrid_data_input = copy.deepcopy(microgrid_data_
            initial[type_nr])
            for entry in microgrid_entries:
```

Note: So far, demand and RE capacity factor timeseries are scaled for entire microgrid categories of

a region. In comparison to the variety of millions of demand and weather curves of large regions, this leads to unrealistically high simultaneity as the number of different timeseries in the model is limited. Thereby, peaks for generation and demand curves get clearly higher leading to overestimated peak load capacity requirements and thus increasing overall system costs. The idea of a quantity number >1 in the selection list was to build different microgrids of the same type with automated timeseries variability to counteract this effect. Due to computational limits, this hasn't been pursued yet but is kept in the script for potential future work. However, in our approach, this increased peaks can be reduced with the applied timeseries aggregation method that has a beneficial smoothing effect on demand curves.

2. Model Connection

Specification of the DS data to the overlying regions by defining unique indices for each parameter and region and the automated definition of a direct connection representing the transformer interface between both system levels:

```
def create_microgrid_data(microgrid_data_input, entry, n, top_region_name):
    ### Parameter Indexing
    microgrid_data_input['site'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=1,
    inplace=True)
    microgrid_data_input['commodity'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=1,
    inplace=True)
    microgrid_data_input['process'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=1,
    inplace=True)
    microgrid_data_input['process_commodity'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=1,
    inplace=True)
    microgrid_data_input['demand'].rename(
        columns={entry: entry + str(n + 1) + '_' + top_region_name},
    level=0, inplace=True)
    microgrid_data_input['supim'].rename(
        columns={entry: entry + str(n + 1) + '_' + top_region_name},
    level=0, inplace=True)
    microgrid_data_input['storage'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=1,
    inplace=True)
    microgrid_data_input['dsm'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=1,
    inplace=True)
    microgrid_data_input['buy_sell_price'].rename(
        columns={entry: entry + str(n + 1) + '_' + top_region_name},
    level=0, inplace=True)
    microgrid_data_input['eff_factor'].rename(
        columns={entry: entry + str(n + 1) + '_' + top_region_name},
    level=0, inplace=True)
    ### for transmission data indexes on two levels must be changed
    microgrid_data_input['transmission'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=1,
    inplace=True)
    microgrid_data_input['transmission'].rename(
        index={entry: entry + str(n + 1) + '_' + top_region_name}, level=2,
    inplace=True)
```

(continues on next page)

(continued from previous page)

```

### Transformer Interface
microgrid_data_input['transmission'].rename(
    index={'top_region_dummy': top_region_name}, level=1, inplace=True)
microgrid_data_input['transmission'].rename(
    index={'top_region_dummy': top_region_name}, level=2, inplace=True)
return microgrid_data_input

```

3. Parameter Scaling

Scaling of parameters with appropriate multipliers (see *How to Determine Multipliers*) to represent the multitude of the distribution systems:

```

def multiplier_scaling(mode, data, microgrid_data_input, microgrid_
    ↳multiplier_list, set_number, type_nr):
    ### determine multiplier for region and microgrid type
    multi = data['transdist_share'].values[0] * microgrid_multiplier_
    ↳list[set_number][type_nr]
    ### base voltage is scaled with the root value of the multiplier_
    ↳for a correct consideration within the voltage rule
    microgrid_data_input['site'].loc[:, 'base-voltage'] *= math.sqrt(multi)
    ### scale other relevant quantities
    microgrid_data_input['commodity'].loc[:, 'max':'maxperhour'] *= multi
    microgrid_data_input['process'].loc[:, ['inst-cap', 'cap-lo', 'cap-up',
    ↳'cap-block']] *= multi
    microgrid_data_input['transmission'].loc[:, ['inst-cap', 'cap-lo',
    ↳'cap-up', 'tra-block']] *= multi
    microgrid_data_input['storage'].loc[:, ['inst-cap-c', 'cap-lo-c', 'cap-
    ↳up-c', 'inst-cap-p', 'cap-lo-p',
    ↳'cap-up-p', 'c-block', 'p-block
    ↳']] *= multi
    microgrid_data_input['dsm'].loc[:, 'cap-max-do':'cap-max-up'] *= multi
    ### if tsam activated postpone demand scaling to reduce number of tsam_
    ↳input timeseries, but still pass demand shift
    if mode['tsam'] == True:
        demand_shift = microgrid_data_input['demand'] * multi
    ### otherwise also scale demand data
    if mode['tsam'] == False:
        microgrid_data_input['demand'] *= multi
        demand_shift = microgrid_data_input['demand']
    return microgrid_data_input, demand_shift

```

Note: Postponement of demand scaling if tsam is active

The timeseries aggregation method that is described in *Time Series Aggregation with Typeperiods* is sensitive to duplicated input timeseries. Therefore, only unique timeseries are handed over as input. All households are defined with the same microgrid templates. If these are scaled before handing them over to the TSA method, duplicate profiles with different scales are not recognized. Therefore, in this case the scaling of the demand is postponed.

4. Scenario Shifting

Demand shifting between scenarios for better comparability:

```
def shift_demand(data, microgrid_data_input, set_number, type_nr, demand_
    shift, loadprofile_BEV, top_region_name,
        mobility_transmission_shift, heat_transmission_shift,
    transdist_eff):
    ### subtract private electricity demand at distribution level
    (increased by tdi efficiency) from transmission level considering line
    losses
    data['demand'].iloc[:, set_number] -= demand_shift.loc[:, pd.
    IndexSlice[:, 'electricity']].sum(axis=1) / transdist_eff
    if data['transdist_share'].values[0] == 1:
        ### store scaled full mobility and heat demand for 100% active
        distribution network for subsequent scenarios
        mobility_transmission_shift[(top_region_name, type_nr)] =
    loadprofile_BEV * demand_shift.loc[:, pd.IndexSlice[:, 'mobility']].
    sum().sum() / transdist_eff
        COP_ts = microgrid_data_input['eff_factor'].loc[:, pd.IndexSlice[:,
    'heatpump_air']].iloc[:, 0].squeeze() #get COP timeseries to transform
    hourly heat to electricity demand
        heat_transmission_shift[(top_region_name, type_nr)] = demand_shift.
    loc[:, pd.IndexSlice[:, 'heat']].sum(axis=1).divide(COP_ts).fillna(0) /
    transdist_eff
    return data, mobility_transmission_shift, heat_transmission_shift
```

Note: The subsequent full shifting process is explained in detail in the *‘CoTraDis’ application guide*

5. RE Profiles

Copy capacity factor timeseries for renewable energy resources from top level region to all microgrids within that region

```
def copy_SupIm_data(data, microgrid_data_input, top_region_name):
    for col in microgrid_data_input['supim'].columns:
        microgrid_data_input['supim'].loc[:, col] = data['supim'].loc[:,
    (top_region_name, col[1])]
    return microgrid_data_input
```

6. Reactive Power Flows

Model new imaginary lines to enable reactive power flow on respective lines with defined resistance:

```
def add_reactive_transmission_lines(microgrid_data_input):
    ### copy transmission lines with resistance to model transmission
    lines for reactive power flows
    reactive_transmission_lines = microgrid_data_input['transmission
    '][microgrid_data_input['transmission'].loc[:, 'resistance'] > 0]
    reactive_transmission_lines = reactive_transmission_lines.copy(deep =
    True)
```

(continues on next page)

(continued from previous page)

```

    reactive_transmission_lines.rename(index={'electricity': 'electricity-
→reactive'}, level=4, inplace=True)
    ### set costs to zero as lines are not really built -
    reactive_transmission_lines.loc[:, 'inv-cost':'var-cost'] *= 0
    ### concat new line data
    microgrid_data_input['transmission'] = pd.concat([microgrid_data_input[
→'transmission'], reactive_transmission_lines], sort=True)
    return microgrid_data_input

```

And Implement reactive power outputs as commodity according to predefined power factors for processes:

```

def add_reactive_output_ratios(microgrid_data_input):
    pro_Q = microgrid_data_input['process'][microgrid_data_input['process
→'].loc[:, 'pf-min'] > 0]
    ratios_elec = microgrid_data_input['process_commodity'].loc[pd.
→IndexSlice[:, :, 'electricity', 'Out'], :]
    for process_idx, process in pro_Q.iterrows():
        for ratio_P_idx, ratio_P in ratios_elec.iterrows():
            if process_idx[2] == ratio_P_idx[1]:
                ratio_Q = ratios_elec.loc[pd.IndexSlice[:, ratio_P_idx[1],
→'electricity', 'Out'], :].copy(deep = True)
                ratio_Q.rename(index={'electricity': 'electricity-reactive
→'}, level=2, inplace=True)
                microgrid_data_input['process_commodity'] = microgrid_data_
→input['process_commodity'].append(ratio_Q)
                microgrid_data_input['process_commodity'] = microgrid_data_
→input['process_commodity']\
                    [~microgrid_data_input['process_commodity'].index.
→duplicated(keep='first')]
    return microgrid_data_input

```

7. Concatenation

Concatenation of the previously processed data from both system levels:

```

def concatenate_with_micros(data, microgrid_data):
    data['site'] = pd.concat([data['site'], microgrid_data['site']],
→sort=True)
    data['commodity'] = pd.concat([data['commodity'], microgrid_data[
→'commodity']], sort=True)
    data['process'] = pd.concat([data['process'], microgrid_data['process
→']], sort=True)
    data['process_commodity'] = pd.concat([data['process_commodity'],
→microgrid_data['process_commodity']], sort=True)
    data['process_commodity'] = data['process_commodity'][~data['process_
→commodity'].index.duplicated(keep='first')]
    data['demand'] = pd.concat([data['demand'], microgrid_data['demand']],
→axis=1, sort=True)
    data['supim'] = pd.concat([data['supim'], microgrid_data['supim']],
→axis=1, sort=True)
    data['transmission'] = pd.concat([data['transmission'], microgrid_data[
→'transmission']], sort=True)
    data['storage'] = pd.concat([data['storage'], microgrid_data['storage
→']], sort=True)

```


(continues on next page)

(continued from previous page)

```
data['dsm'] = pd.concat([data['dsm'], microgrid_data['dsm']], sort=True)
data['buy_sell_price'] = pd.concat([data['buy_sell_price'], microgrid_
↪data['buy_sell_price']], axis=1, sort=True)
data['eff_factor'] = pd.concat([data['eff_factor'], microgrid_data[
↪'eff_factor']], axis=1, sort=True)
return data
```

8. Workflow

The workflow of all previously described `transdisthelper.py` implementation is illustrated below:

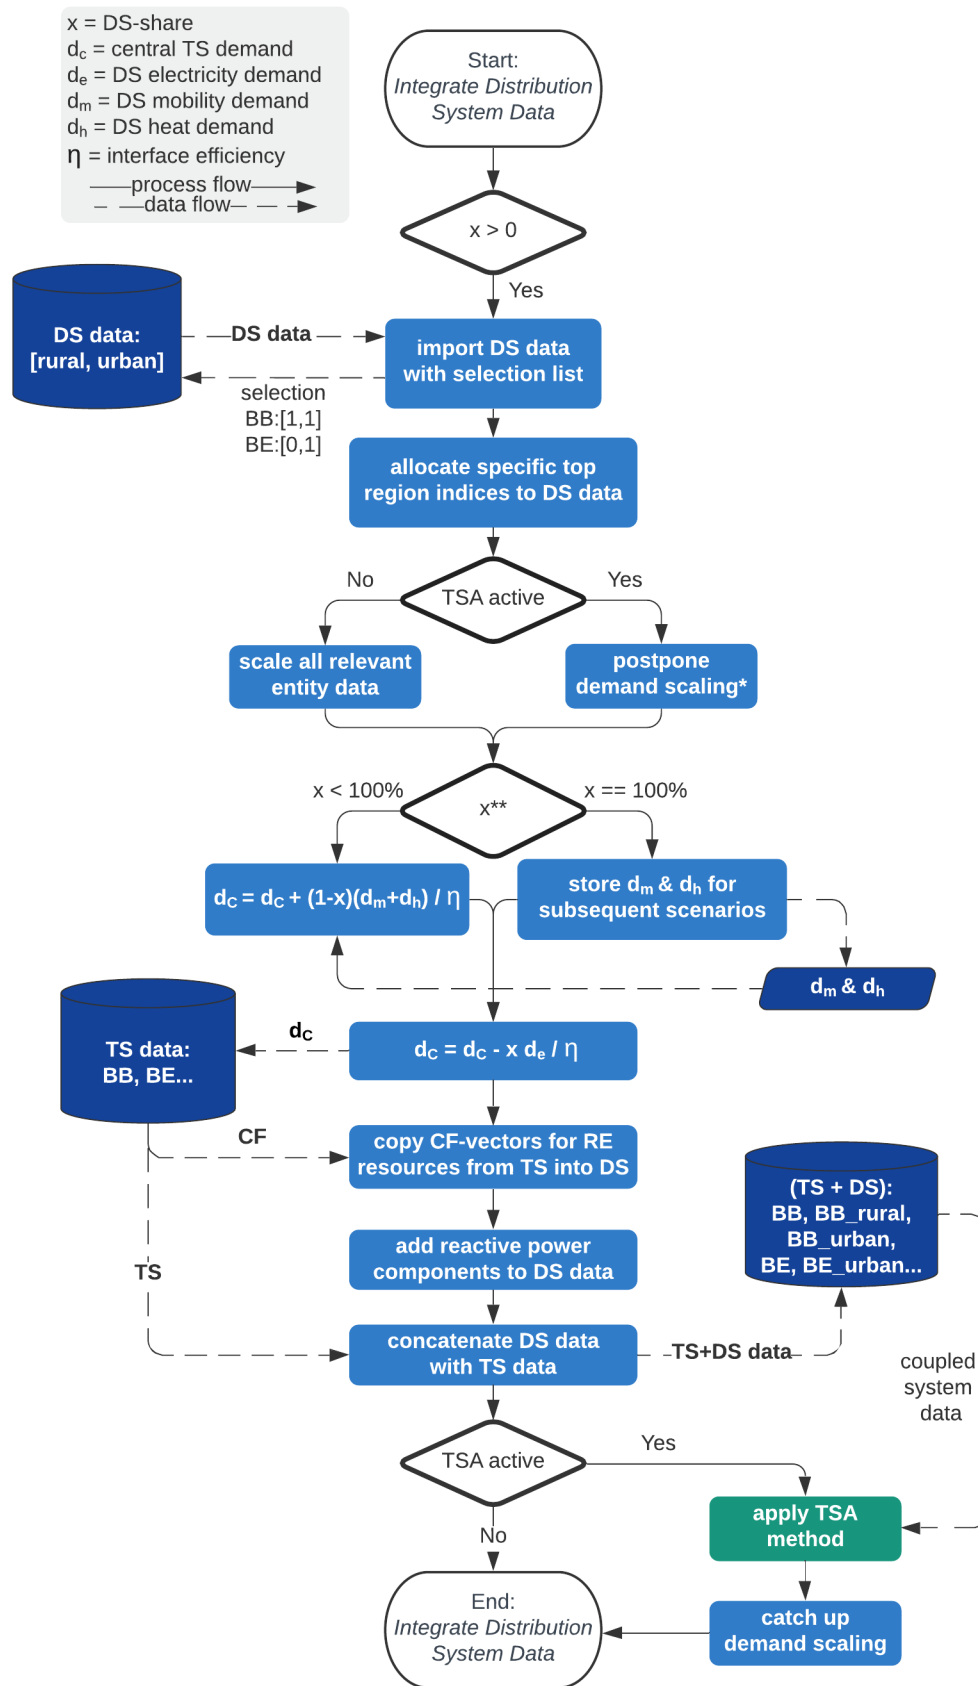

Time Series Aggregation with Typeperiods

Typeperiod Motivation

The type period module has been adapted into the urbs framework by Daniel Zinsmeister and modified to fit into our approach as described below. It allows to scale selected periods to represent the entire year. In energy system models it is popular to do so as there are recurring patterns in relevant timeseries such as demand or solar irradiation profiles. For instance, typical periods for summer and winter time can be chosen and scaled with the corresponding incidence of expected summer/winter periods. Thereby, economic (costs) and environmental (emissions) effects can be scaled adequately.

Approach with the 'tsam' Method

Hereby, the challenge is to choose the most representative period of a season. The timestep selection must hold for all input timeseries. Considering only one solar irradiation curve when defining two typical periods for summer and winter, it is possible to manually choose the best fitting weeks within the year. However, even a simplified model of a country considers approximately 100 distinct profiles. Hence, it is not possible to manually choose the most suitable representative periods and a mathematical and automated method is necessary instead. Therefore, to choose the best fitting typeperiods an open source python package called tsam is used, that applies machine learning methods and has been developed by Leander Kotzur, Maximilian Hoffmann, Peter Markewitz, Martin Robinius and Detlef Stolten. To understand the tsam procedure in detail see their provided [tsam documentation](#). Summarized, a predefined number of type periods with a selected number of hours per period is calculated to optimally represent the original data for all timeseries simultaneously. This is realized by optimizing cluster groups with the Root-Mean-Squared-Error (RMSE) as objective functional value. Thereby, redundant data are minimized and thereby computational complexity can be substantially decreased.

In our approach before giving the timeseries data to the tsam algorithm, for all redundant profiles, a 'Python' dictionary is created to remember the equal profiles which have been handed over. Next all duplicates are deleted. By doing so the number of input timeseries in our approach could be reduced from 1638 to 95.

```
def run_tsam(data, noTypicalPeriods, hoursPerPeriod, cross_scenario_data):
    ### bring together all time series data
    time_series_data = pd.concat([data['demand'], data['supim'], data['buy_
→sell_price'],
                                data['eff_factor']], axis=1, sort=True)

    ### create dict
    equal_col_dict = dict()
    for col1 in time_series_data.columns:
        time_series_data2 = time_series_data.drop(columns = col1)
        for col2 in time_series_data2.columns:
            if time_series_data[col1].equals(time_series_data2[col2]):
                equal_col_dict[col1] = col2
                break
    ### drop duplicate timeseries
    time_series_data = time_series_data.T.drop_duplicates().T
```

This dictionary is used after the application of the timeseries aggregation to allocate the results to all original profiles.

Enabling Seasonal Storage Solutions

The motivation to apply typical periods is to weight cluster periods based on their total incidence number. The explicit chain of periods and thus the transition between distinct periods is not considered. Thereby, the overall number of periods to model keeps low and thus the computational complexity is reduced. Despite, the disadvantage is that the possibility of energy exchange between periods is disregarded. As a consequence, storage components must be modelled with an additional constraint denoted as cyclicity condition setting all period's final storage SOC's equal to the initial values.

```


### original timeset for cyclicity rule
m.t_endofperiod = pyomo.Set(
    within=m.t,
    initialize=t_endofperiod_list,
    ordered=True,
    doc='timestep at the end of each timeperiod')

### cyclicity constraint
m.res_storage_state_cyclicity_typeperiod = pyomo.Constraint(
    m.t_endofperiod, m.sto_tuples,
    rule=res_storage_state_cyclicity_typeperiod_rule,
    doc='storage content initial == storage content at the end of each_
→timeperiod')

### cyclicity rule without tsam
def res_storage_state_cyclicity_typeperiod_rule(m, t, stf, sit, sto, com):
    return (m.e_sto_con[m.t[1], stf, sit, sto, com] == m.e_sto_con[t, stf,
→sit, sto, com])

```

The resulting main disadvantage is that long-term storage solutions that are essential for RE-dominant energy systems cannot be considered appropriately. Therefore, we apply a time series aggregation method with typical weeks combined with an additional storage constraint that enables the exchange of energy between consecutive, alternating periods (for instance the type periods A and B). This relaxes the cyclicity condition within a given type period, i.e. a total SOC change within a given type period A is allowed. The basic idea is illustrated below for four typical weeks:

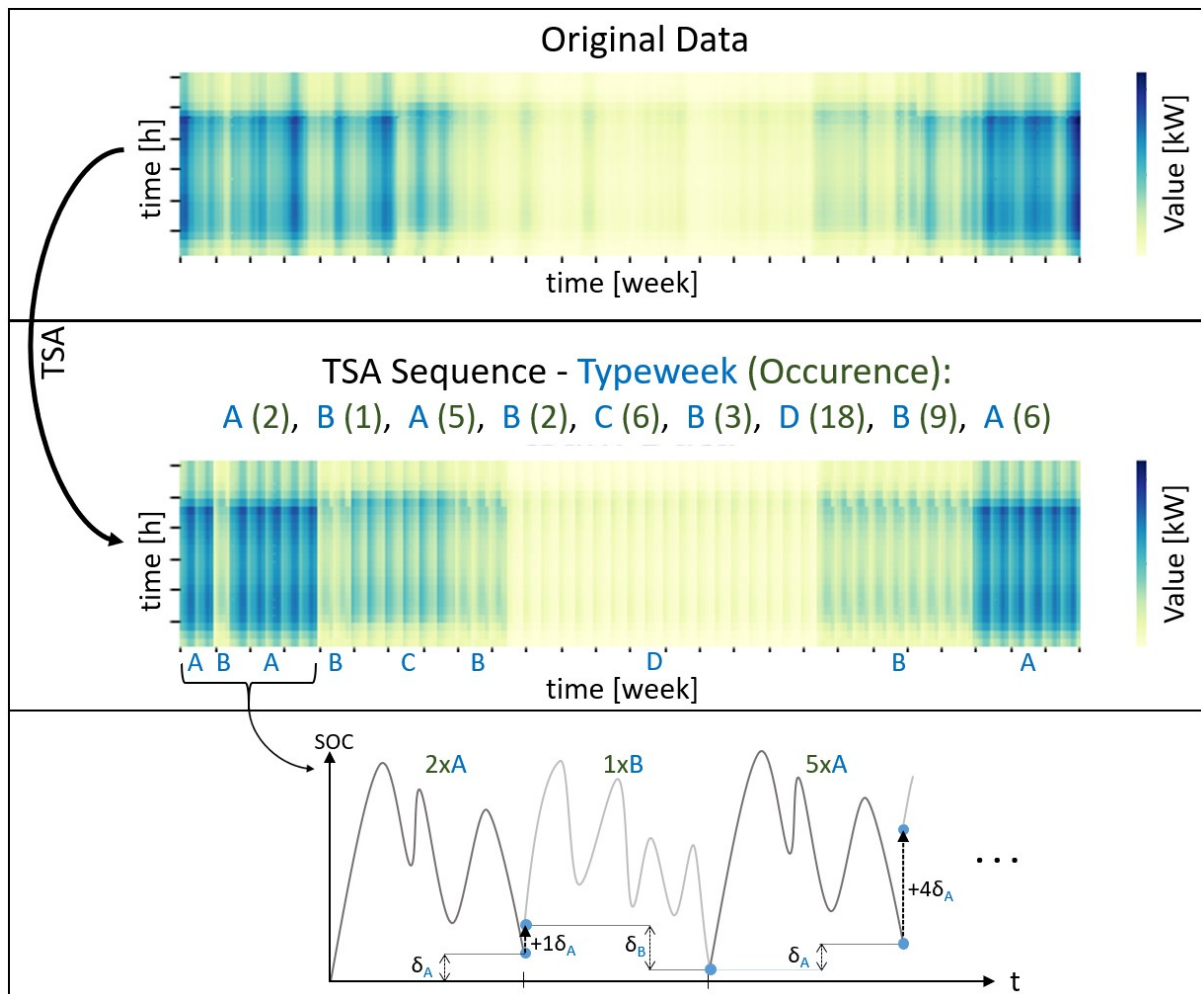

The definition of required sets, variables, constraints and rules to implement this idea are presented below:

```

### sets
m.t_endofperiod = pyomo.Set(
    within=m.t,
    initialize=t_endofperiod_list,
    ordered=True,
    doc='timestep at the end of each timeperiod')
m.subsequent_typeperiods = pyomo.Set(
    within=m.t * m.t,
    initialize=subsequent_typeperiods_list,
    ordered=True,
    doc='subsequent timesteps between two typeperiods')
m.start_end_typeperiods = pyomo.Set(
    within=m.t * m.t,
    initialize=start_end_typeperiods_list,
    ordered=True,
    doc='start and end of each modeled typeperiod as tuple')

### SOC variable
m.deltaSOC = pyomo.Var(
    m.t_endofperiod, m.sto_tuples,
    within=pyomo.Reals,
    doc='Variable to describe the delta of a storage within each period')

```

(continues on next page)

(continued from previous page)

```

### constraints
### constraint to describe the SOC difference of a storage within a
↳repeating period A
m.res_delta_SOC = pyomo.Constraint(
    m.start_end_typeperiods, m.sto_tuples,
    rule=res_delta_SOC,
    doc='delta_SOC_A = weight * (SOC_A_tN - SOC_A_t0)')

### SOC constraint for two consecutive typeperiods A and B
m.res_typeperiod_delta_SOC = pyomo.Constraint(
    m.subsequent_typeperiods, m.sto_tuples,
    rule=res_typeperiod_deltaSOC_rule,
    doc='SOC_B_t0 = SOC_A_t0 + delta_SOC_A')

### new ciclycity constraint for typeperiods
m.res_storage_state_cyclicity_typeperiod = pyomo.Constraint(
    m.sto_tuples,
    rule=res_storage_state_cyclicity_rule_typeperiod,
    doc='storage content end >= storage content start - deltaSOC[last_
↳typeperiod]')

### rules
### SOC rule for each repeating typeperiod
def res_delta_SOC(m, t_0, t_end, stf, sit, sto, com):
    return ( m.deltaSOC[t_end, stf, sit, sto, com] ==
            (m.typeperiod_weights[t_end] - 1) * (m.e_sto_con[t_end, stf,
↳sit, sto, com]
            - m.e_sto_con[t_0, stf, sit, sto, com]))

### new storage rule using tsam considering the delta SOC per repeating
↳typeperiod
def res_typeperiod_deltaSOC_rule(m, t_A, t_B, stf, sit, sto, com):
    return (m.e_sto_con[t_B, stf, sit, sto, com] ==
            m.e_sto_con[t_A, stf, sit, sto, com] + m.deltaSOC[t_A, stf,
↳sit, sto, com])

### new ciclycity rule for typeperiods
def res_storage_state_cyclicity_rule_typeperiod(m, stf, sit, sto, com):
    return (m.e_sto_con[m.t[len(m.t)], stf, sit, sto, com] >=
            m.e_sto_con[m.t[1], stf, sit, sto, com] - m.deltaSOC[m.t[len(m.
↳t)], stf, sit, sto, com])

```

‘CoTraDis’ application guide

This section serves as a guide for those who would like to use the CoTraDis module. First the adjusted runme file is introduced. Next, special input parameters to consider are presented. Finally, the default scenario framework is discussed in order to enable you to define own model scenarios.

The script starts with the specification of the input files. The input folder must be located in the same folder as the `run_transdist.py` script. In this folder the main transmission system file is located including another folder that contains input files for each desired microgrid type. The desired input files to be imported must be defined at the beginning of the script

```
input_files = 'Transmission_Level.xlsx' # for single year file name, for_
→intertemporal folder name
microgrid_files = ['Microgrid_rural_A.xlsx', 'Microgrid_urban_A.xlsx']
```

Then the result name and the result directory is set

```
result_name = 'Trans-Dist'
```

Next, the objective function to be minimized by the model is determined (options: 'cost' or 'CO2')

```
# objective function
objective = 'cost' # set either 'cost' or 'CO2' as objective
```

and the solver to use must be chosen. Gurobi is our predefined solver - to use it an academic license must be downloaded at the [Gurobi website](#) after creating an account.

```
# Choose Solver (cplex, glpk, gurobi, ...)
solver = 'gurobi'
```

To apply time series aggregation methods (tsam) the number of typical periods and the length of the periods must be defined:

```
# input data for tsam method
noTypicalPeriods = 4
hoursPerPeriod = 168
```

Watch out! An increasing number of typeperiods crucially influences the computational load due to the introduced seasonal storage constraint (all subsequent alternating typeperiods must be modeled). Evidence has shown, that especially at the beginning when increasing the *noTypicalPeriods* parameter, the computational load increases rapidly. For higher numbers, the constellation of subsequent weeks varies which can even result in lower weeks to model (noTypicalPeriods : modeledWeeks - 2 : 3, 4 : 9, 6 : 14, 8 : 18, 10 : 21, 12 : 20). These values may change for each individual model with its constellation of timeseries for intermittent resources and demand.

If you don't use tsam you must choose the time range to be modeled (default of 8760 hours for the entire year)

```
# simulation timesteps
(offset, length) = (0, 8760) # time step selection
```

Remarks on Input Data

In this section input data that must be additionally considered in the input excel sheet are listed to simplify the application for users:

Transmission System Input File:

Sheet "Global":

- *transDist* parameter to concatenate distribution system data: 1 or 0
- *tsam* parameter: 1 or 0

Sheet “Site”:

- *microgrid setting* to select desired microgrids per region: list
- *multiplier* to scale chosen microgrids: list

Distribution System Input File:**Sheet “Site”:**

- *base voltage* of the distribution system level: value
- *ref-node* to indicate reference node with transformer interface: 1 or 0
- *min/max-voltage* to define permissible voltage range: value

Note: Permissible voltage range must be adjusted to the length of microgrid branches

In our case study for German distribution systems we identified a possible voltage range from 0.95 to 1.03 per unit. These values are representative for actual grids which have more nodes that can be modeled. Therefore, to get a meaningful voltage constraint, the range must be appropriately reduced.

Sheet “Commodity”:

- commodities must be defined for all nodes that are desired to be constrained by a vertex rule of the commodity (for the transmission of the commodity also if no processes of the commodity are defined)

Sheet “Process”:

- the power factor parameter *pf-min*: value
- declare own slack process for better debugging on distribution system level
- if the expansion of distribution system components is intended to be included into the optimization, price parameters must be defined (e.g. when comparing two different technologies to cover the heat demand)

Sheet “Transmission”:

- **the impedance parameters are determining for the power flow model to be applied (resistance, reactance):**
 - (#N/A, #N/A) : transport model
 - (#N/A, >0) : DCPF model
 - (>0, >0) : LinDistFlow model
- transmission distribution interface transformer parameter must be chosen carefully (similar to voltage range determination)

Sheet “SupIm”:

- timeseries for intermittent ressources are automatically taken from the regions the microgrids are defined in. Hence timeseries here are defined with zero vectors.

How to Determine Multipliers

The residential quantities such as demand and capacity potentials have been defined for the entire country in only two microgrids with 25 nodes together. Obviously, to describe the entire country they must be scaled. The multipliers must be carefully derived to represent the desired system. The default microgrids and the related multipliers have been derived to include all residential buildings in Germany as follows:

We categorized the DS into two possible microgrid modules: Living areas differ in some aspects such as population density, PV potentials and mobility requirements. Therefore two general areas are defined: rural (r) and urban (u). The population distribution by regions is categorized into these categories by summing up all people living in cities greater than 50 thousand inhabitants to the urban population P_u for each region. The remaining population is allocated to the rural population P_r . To represent the correct ratio of single family houses (S) to multi apartment houses (M) within the microgrids the range of house category shares $x = \frac{\zeta_S}{\zeta_M}$ for rural and urban areas averaged for Germany are estimated (no detailed information about the region-wise distribution of inhabitants by S and M could be found).

To meet the exact number of S and M in Germany the defined microgrid must be scaled appropriately. Accordingly, two parameters are aimed to be determined: the multipliers for each region to scale the defined microgrid and the best fitting house category ratio x within the given range. As the given rural and urban population per region on one side is given as a quantity of people but on the other side the ratio x is given for house categories, the latter entity must be converted to a ratio of people shares $y = \frac{\rho_S}{\rho_M}$. The assumptions of two persons living in an average German household and 7 households per apartment house are used to determine the number of residents per S ($\epsilon_S = 2$) and M ($\epsilon_M = 14$). Next, the population ratio can be calculated:

$$\frac{\rho_S}{\rho_M} = x \frac{\epsilon_S}{\epsilon_M} = \underbrace{\frac{\zeta_S}{\zeta_M} \frac{\epsilon_S}{\epsilon_M}}_{\alpha}$$

Combining $\rho_S = \alpha \rho_M$ and $\rho_S + \rho_M = 1$ yields:

$$\rho_S = \frac{\alpha}{1 + \alpha}$$

Next, the most representative value of x is determined by varying it until the resulting total quantity of S and M for overall Germany is as close as possible to values derived with a second top-down approach: The total number of residential buildings in Germany is taken and divided into both house categories. Finally, the resulting share ρ_S can be multiplied with the population P of the respective area to get the number of people P_S living in single family houses for both area types. To get the required multipliers μ , P_S needs to be divided by ϵ_S and the defined number of S in the respective microgrid category:

$$\mu = \frac{P_S}{\epsilon_S S}$$

Only this parameter μ_S is required, as the ratio between S and M is determined with x .

Note: Multipliers must fit to the defined microgrids and the research question

The modular definition of the microgrids and the scaling can be freely performed depending on the research topic. However, please keep in mind that the interdependency between microgrid definition and multiplier derivation is important to finally depict the desired energy system as realistically as possible. The introduced approach to determine the multipliers may not be suitable for different microgrid structures!

Remarks on the Scenario Shifting Approach

When transmission and distribution demand data are combined, special care must be taken to avoid a double counting. For instance, the default electricity demand curve per German regions already include the residential electricity consumption. In the conducted study, a central research question was to analyze the impact of increasing shares of active distribution grids. Therefore, when introducing distribution systems with demand curves for households the hourly total distribution system demand within a region must be subtracted from the respective transmission system demand.

To secure comparability between scenarios, the total demand must be constant. Thus, if the distribution network is only partly modeled as active grid, the demand must be shifted between both system levels. For the basic electricity demand, this is implemented in the `transdist.py` module with the `shift_demand` function that subtracts less from the top region demand with decreasing distribution network shares (*transdist_share*). When multiple scenarios are modeled, it is recommended to run first the 100% active distribution grid scenario, as thereby the maximum demand for mobility and heat can be stored to be used in subsequent scenarios with lower *transdist_shares*.

```
### Shift demand between scenarios for better comparability
def shift_demand(data, microgrid_data_input, set_number, type_nr, demand_
    ↳ shift, loadprofile_BEV, top_region_name,
        mobility_transmission_shift, heat_transmission_shift,
    ↳ transdist_eff):
    ### subtract private electricity demand at distribution level
    ↳ (increased by tdi efficiency) from transmission level considering line
    ↳ losses
    data['demand'].iloc[:, set_number] -= demand_shift.loc[:, pd.
    ↳ IndexSlice[:, 'electricity']].sum(axis=1) / transdist_eff

    if data['transdist_share'].values[0] == 1:
        ### store scaled full mobility and heat demand for 100% active
    ↳ distribution network for subsequent scenarios
        mobility_transmission_shift[(top_region_name, type_nr)] =
    ↳ loadprofile_BEV * demand_shift.loc[:, pd.IndexSlice[:, 'mobility']].
    ↳ sum().sum() / transdist_eff
        COP_ts = microgrid_data_input['eff_factor'].loc[:, pd.IndexSlice[:,
    ↳ 'heatpump_air']].iloc[:,0].squeeze() #get COP timeseries to transform
    ↳ hourly heat to electricity demand
        heat_transmission_shift[(top_region_name, type_nr)] = demand_shift.
    ↳ loc[:, pd.IndexSlice[:, 'heat']].sum(axis=1).divide(COP_ts).fillna(0) /
    ↳ transdist_eff
    return data, mobility_transmission_shift, heat_transmission_shift
```

Note: Transformer losses at the interface are important for scenario comparability

When modeling a fully active distribution grid a higher share of the demand is modeled within the distribution system. Having energy flows between both systems and a transformer at the interface that is modeled with losses, the total energy that is required by the energy system increases. Therefore, to compare equal energy requirements for all scenarios, these losses are considered with the ‘*transdist_eff*’ parameter in the shifting processes.

In comparison, the central demand does not include charging of battery electric vehicles or the widespread application of heatpumps. Hence, for the mobility and heat demand the scenario module has been extended with a function to consider this. The *variable_distribution_share* function on one

side shifts the inflexible demand curves to the transmission system level. On the other side, it ensures that the PV-potentials (depending on the distribution grid input parameters) are constant for all scenarios.

```
def variable_distribution_share(data, cross_scenario_data, transdist_
→share):
    data['transdist_share'] = pd.Series([transdist_share]) # defined as_
→series to avoid validation error
    if transdist_share < 1:
        if bool(cross_scenario_data):
            data['process'].loc[pd.IndexSlice[:, :, 'PV_utility_rooftop'],
→'cap-up'] =
            data['process'].loc[pd.IndexSlice[:, :, 'PV_utility_rooftop'],
→'cap-up'].values \
            + (1 - transdist_share) * cross_scenario_data['PV_cap_shift'].
→values
            ### read additional demand (BEV, Heat) from cross_scenario data
            additional_demand_mobility = cross_scenario_data['mobility_
→transmission_shift']
            additional_demand_heat = cross_scenario_data['heat_
→transmission_shift']
            ### add additional electricity demand for mobility and heat on_
→transmission level
            for col in data['demand']:
                if col[0] in list(additional_demand_mobility.columns):
                    data['demand'].loc[:, col] += additional_demand_mobility.
→loc[:, col[0]] * (1 - transdist_share)
                if col[0] in list(additional_demand_heat.columns):
                    data['demand'].loc[:, col] += additional_demand_heat.loc[:,
→col[0]] * (1 - transdist_share)
            return data, cross_scenario_data
```

The responsible *transdist_share* is determined in the scenario module, by adjusting the respective parameter (e.g. for a 66% active distribution grid):

```
def transdist66(data, cross_scenario_data):
    data['global_prop'].loc[pd.IndexSlice[:, 'TransDist'], 'value'].
→iloc[0] = 1
    data, cross_scenario_data = variable_distribution_share(data, cross_
→scenario_data, 0.66)
    return data, cross_scenario_data
```

Before using the discussed scenario framework you should answer yourself the following question:

Do you want to consider different shares for active distribution systems?

- Yes - Than you need to fully understand the scenario implementations as described above.
- No - Than you basically need to know that using the default framework, the normal electricity demand needs to be defined within the transmission system demand timeseries, but additional electricity demand from sector coupling must not be included.

Features

- [urbs](#) is a linear programming optimization model for multi-commodity energy systems, their sizing, development and utilization.
- It finds the minimum cost energy system to satisfy given demand timeseries for possibly multiple commodities (e.g. electricity, heat).
- By default, operates on hourly-spaced timesteps (configurable) and can be used for intertemporal optimization.
- Thanks to [pandas](#), complex data analysis code is short and extensible.
- The model itself is quite small thanks to relying on the [Pyomo](#) package.
- [urbs](#) includes reporting and plotting functions for rapid scenario development.

3.1 2019-03-13 Version 1.0

- Maintenance: Modularity (only features which are used are build)
- Maintenance: New structure of documentation
- Feature: Time variable efficiency
- Feature: Objective function can be changed to CO2
- Feature: Intertemporal feature (expansion between years)
- Feature: Input validation (having easier to understand error messages due to Excel file)
- Feature: Reconstruction of partial feature
- Feature: Global constraints instead of Hacks
- Bugfixes: Many

3.2 2017-01-13 Version 0.7

- Maintenance: Model file `urbs.py` split into subfiles in folder `urbs`
- Feature: Usable area in site implemented as possible constraint
- Feature: Plot function (and `get_timeseries`) now support grouping of multiple sites
- Feature: Environmental commodity costs (e.g. emission taxes or other pollution externalities)
- Bugfix: column *Overproduction* in report sheet did not respect DSM

3.3 2016-08-18 Version 0.6

- *Demand Side Management Constraints* added
- *Process Constraints for partial operation* added
- Various fixes in examples, docs and tutorials for Pyomo 4/Python 3 changes

3.4 2016-02-16 Version 0.5

- Support for Python 3 added
- Support for Pyomo 4 added, while maintaining Pyomo 3 support. Upgrading to Pyomo 4 is advised, as support will be dropped with the next release to support new features.
- New feature: maximal power gradient for conversion processes
- Documentation: *buyselldoc* (expired) long explanation for *Buy* and *Sell* commodity types
- Documentation: *Model Implementation* full listing of sets, parameter, variables, objective function and constraints in mathematical notation and textual explanation
- Documentation: updated installation notes in [README.md](#)
- Plotting: automatic sorting of time series by variance makes it easier to read stacked plots with many technologies


3.5 2015-07-29 Version 0.4

- Additional commodity types *Buy* and *Sell*, which support time-dependent prices.
- Persistence functions *load* and *save*, based on pickle, allow saving and retrieving input data and problem instances including results, for later re-plotting or re-analysis without having to solve them again.
- Documentation: *workflow* tutorial added with example “Newsealand”


3.6 2014-12-05 Version 0.3

- Processes now support multiple inputs and multiple output commodities.
- As a consequence `plot()` now plots commodity balance by processes, not input commodities.
- urbs now supports input files with only a single site; simply delete all entries from the ‘Transmission’ spreadsheet and only use a single site name throughout your input.
- Moved hard-coded ‘Global CO2 limit’ constraint to dedicated “Hacks” spreadsheet, while the constraint is `add_hacks()`.
- More docstrings and comments in the main file `urbs.py`.

This is a typical result plot created by `urbs.plot()`, showing electricity generation and storage levels in one site over 10 days (240 time steps):

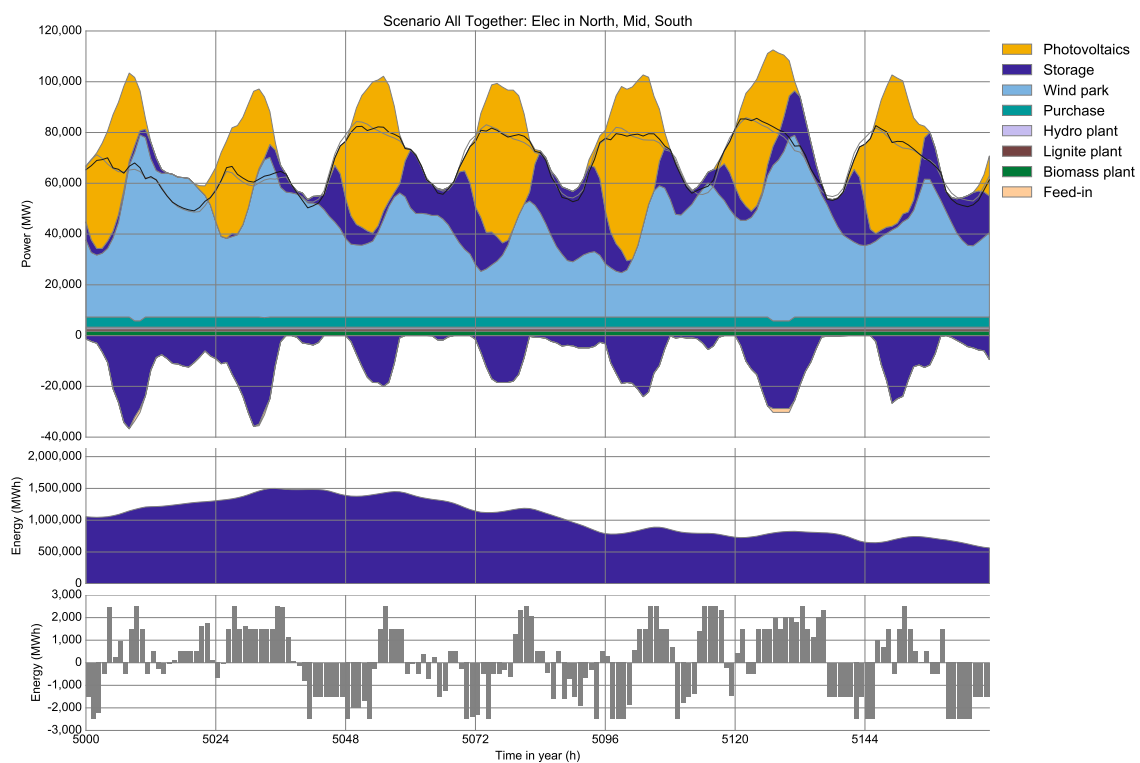

An exemplary comparison script `comp.py` shows how one can create automated cross-scenario analyses with very few lines of `pandas` code. This resulting figure shows system costs and generated electricity by energy source over five scenarios:

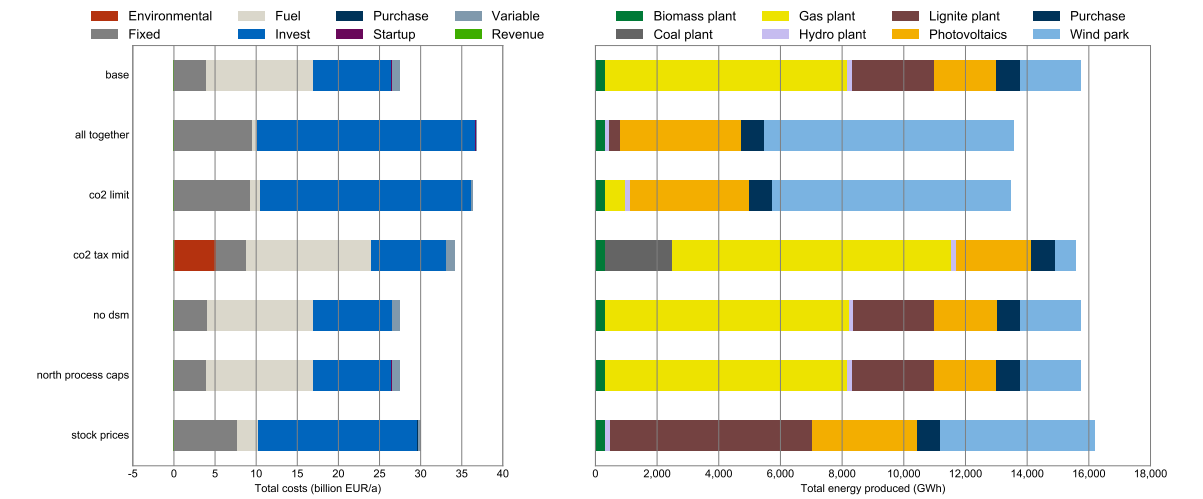

CHAPTER 5

Dependencies

- [Python](#) versions 2.7 or 3.x are both supported.
- [pyomo](#) for model equations and as the interface to optimisation solvers (CPLEX, GLPK, Gurobi, ...). Version 4 recommended, as version 3 support (a.k.a. as `coop.pyomo`) will be dropped soon.
- [matplotlib](#) for plotting due to its capability to customise everything.
- [pandas](#) for input and result data handling, report generation
- Any solver supported by pyomo; suggestion: [GLPK](#)

U

urbs, [12](#)

C

`commodity_subset()` (*in module urbs*), 63

U

`urbs` (*module*), 1, 3, 5, 12, 20, 22, 23, 28, 31, 35,
38, 39, 42, 49, 68, 77, 89, 96